
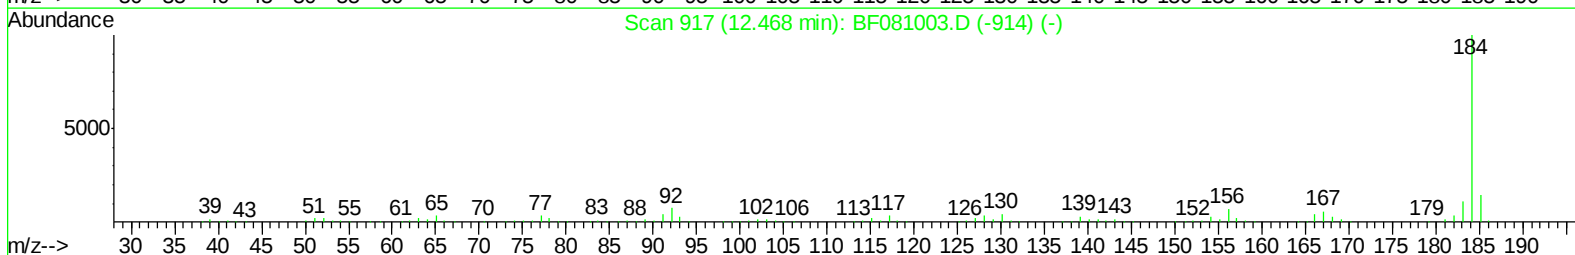
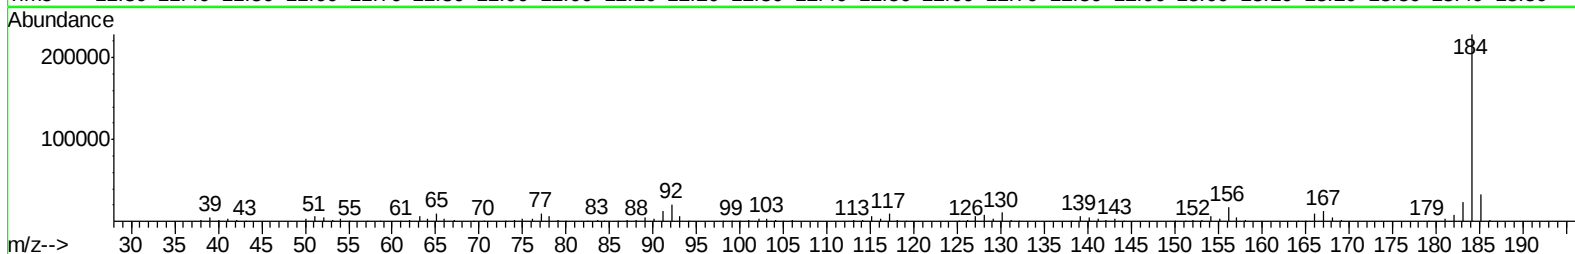


Data Path : Z:\HPCHEM1\BNA_F\Data\BF081715\
Data File : BF080999.D
Acq On : 17 Aug 2015 11:48
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 04:13:18 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 03:32:45 2015
Response via : Initial Calibration

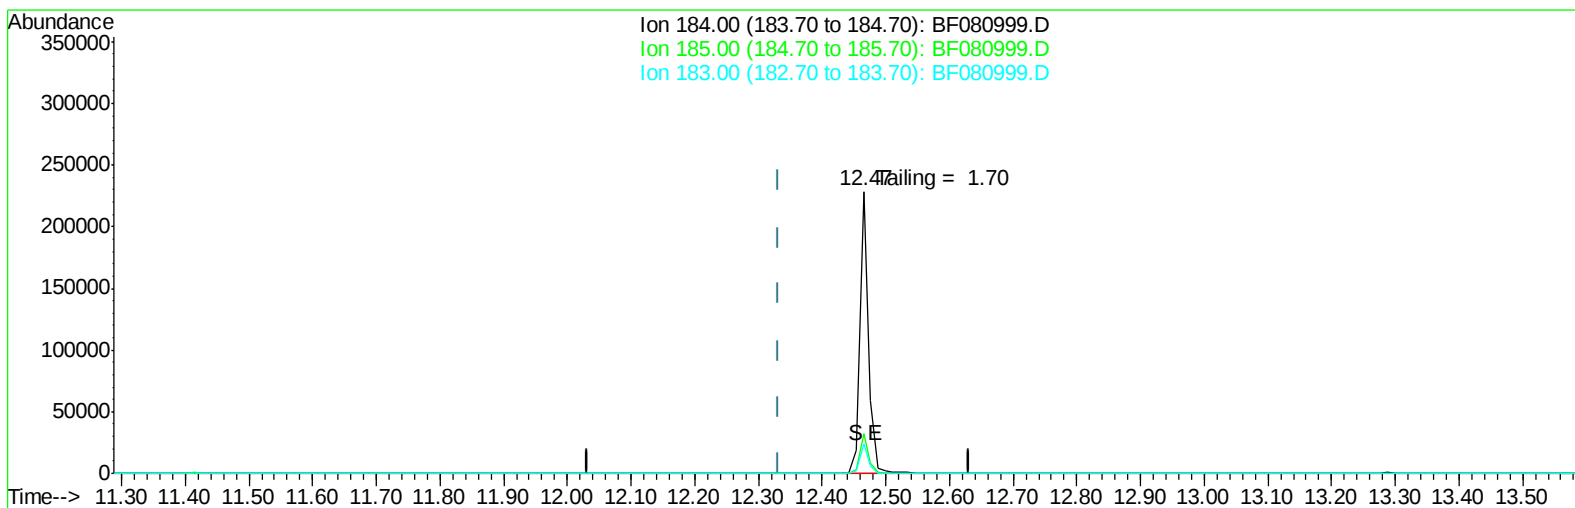

TIC: BF080999.D

(76) Benzidine




12.465min (+0.133) 0.00ng

response 217555

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.27
183.00	11.10	10.67
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF081715\  
Data File : BF080999.D  
Acq On    : 17 Aug 2015  11:48  
Operator  : UM/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Aug 28 04:13:18 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 03:32:45 2015
Response via : Initial Calibration

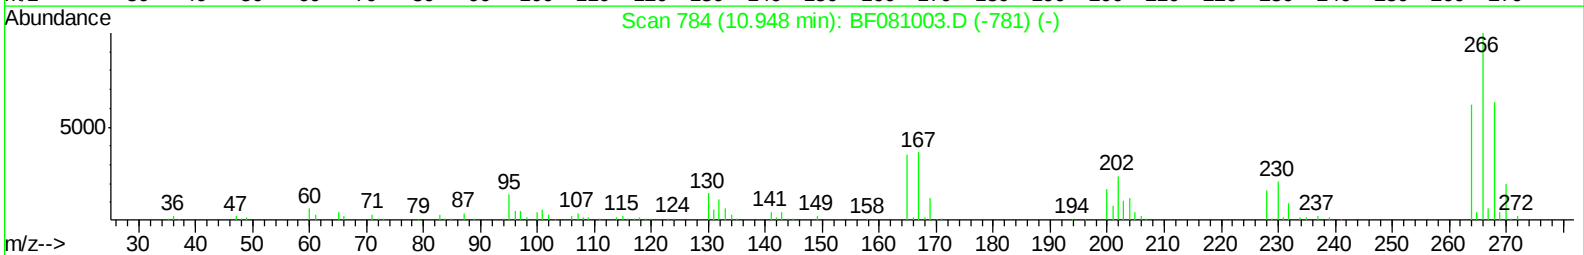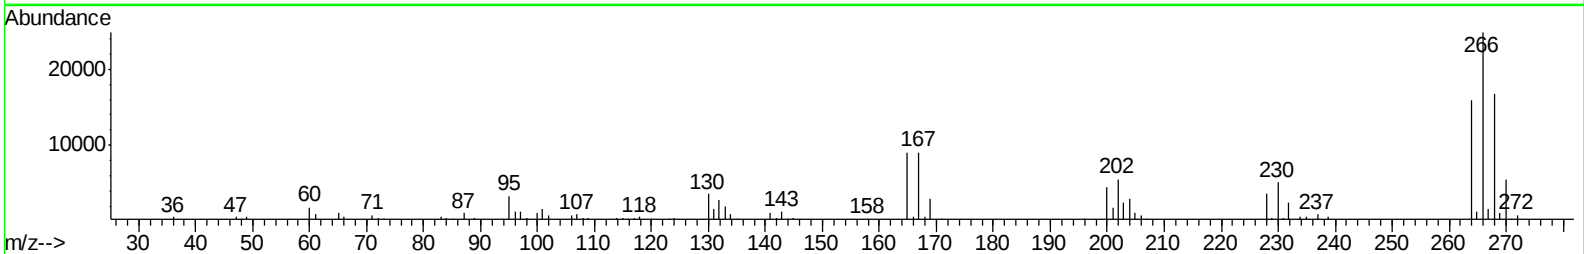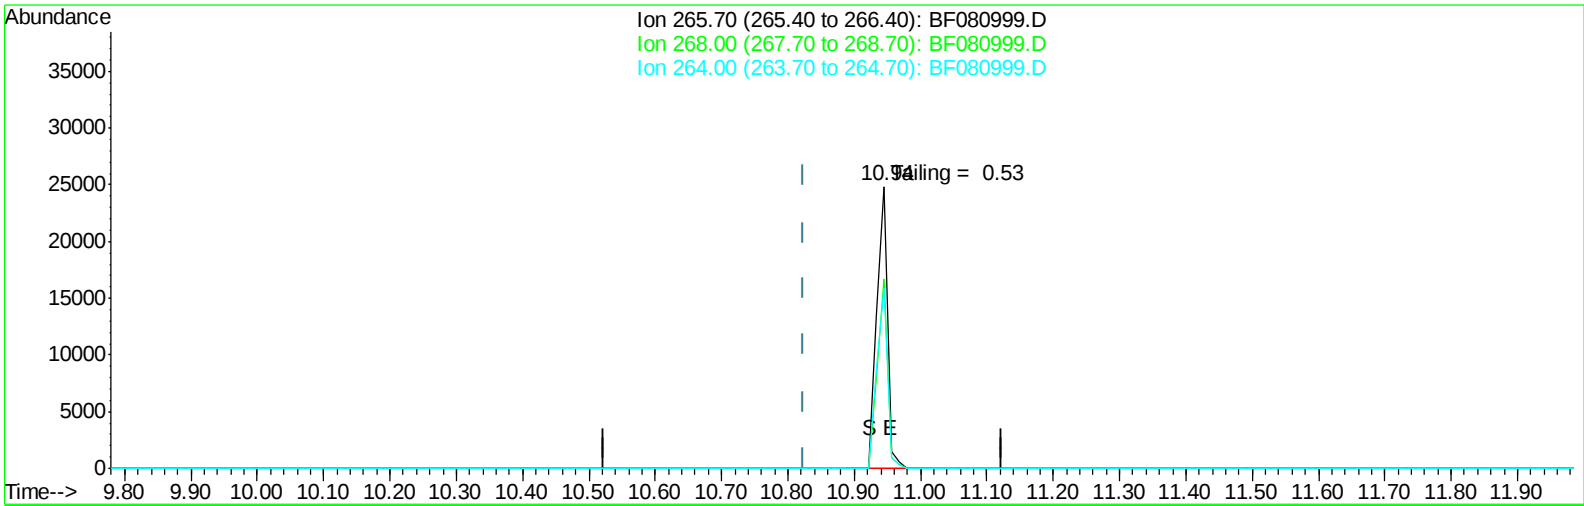

TIC: BF080999.D

(69) Pentachlorophenol (C)

10.945min (+0.121) 0.00ng

response 27572

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	67.39
264.00	63.20	64.04
0.00	0.00	0.00