

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081715\
 Data File : BF081031.D
 Acq On : 18 Aug 2015 5:51
 Operator : UM/IZ
 Sample : G3290-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 2A(0-2)-4

Quant Time: Aug 18 06:53:36 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 17:57:25 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.63	152	59825	20.00	ng	0.00
21) Naphthalene-d8	7.91	136	208351	20.00	ng	0.00
38) Acenaphthene-d10	9.66	164	90694	20.00	ng	0.00
63) Phenanthrene-d10	11.13	188	157155	20.00	ng	0.00
75) Chrysene-d12	13.75	240	125210	20.00	ng	0.00
86) Perylene-d12	15.11	264	90991	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.20	112	383263	96.36	ng	0.01
7) Phenol-d6	6.27	99	506413	97.58	ng	0.01
23) Nitrobenzene-d5	7.20	82	349042	76.53	ng	0.01
41) 2,4,6-Tribromophenol	10.44	330	73071	92.95	ng	0.00
44) 2-Fluorobiphenyl	8.99	172	458416	66.23	ng	0.00
78) Terphenyl-d14	12.72	244	321360	55.02	ng	0.01
Target Compounds						
49) Dimethylphthalate	9.39	163	91011	12.18	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081715\
Data File : BF081031.D
Acq On : 18 Aug 2015 5:51
Operator : UM/IZ
Sample : G3290-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
2A(0-2)-4

Quant Time: Aug 18 06:53:36 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 17:57:25 2015
Response via : Initial Calibration

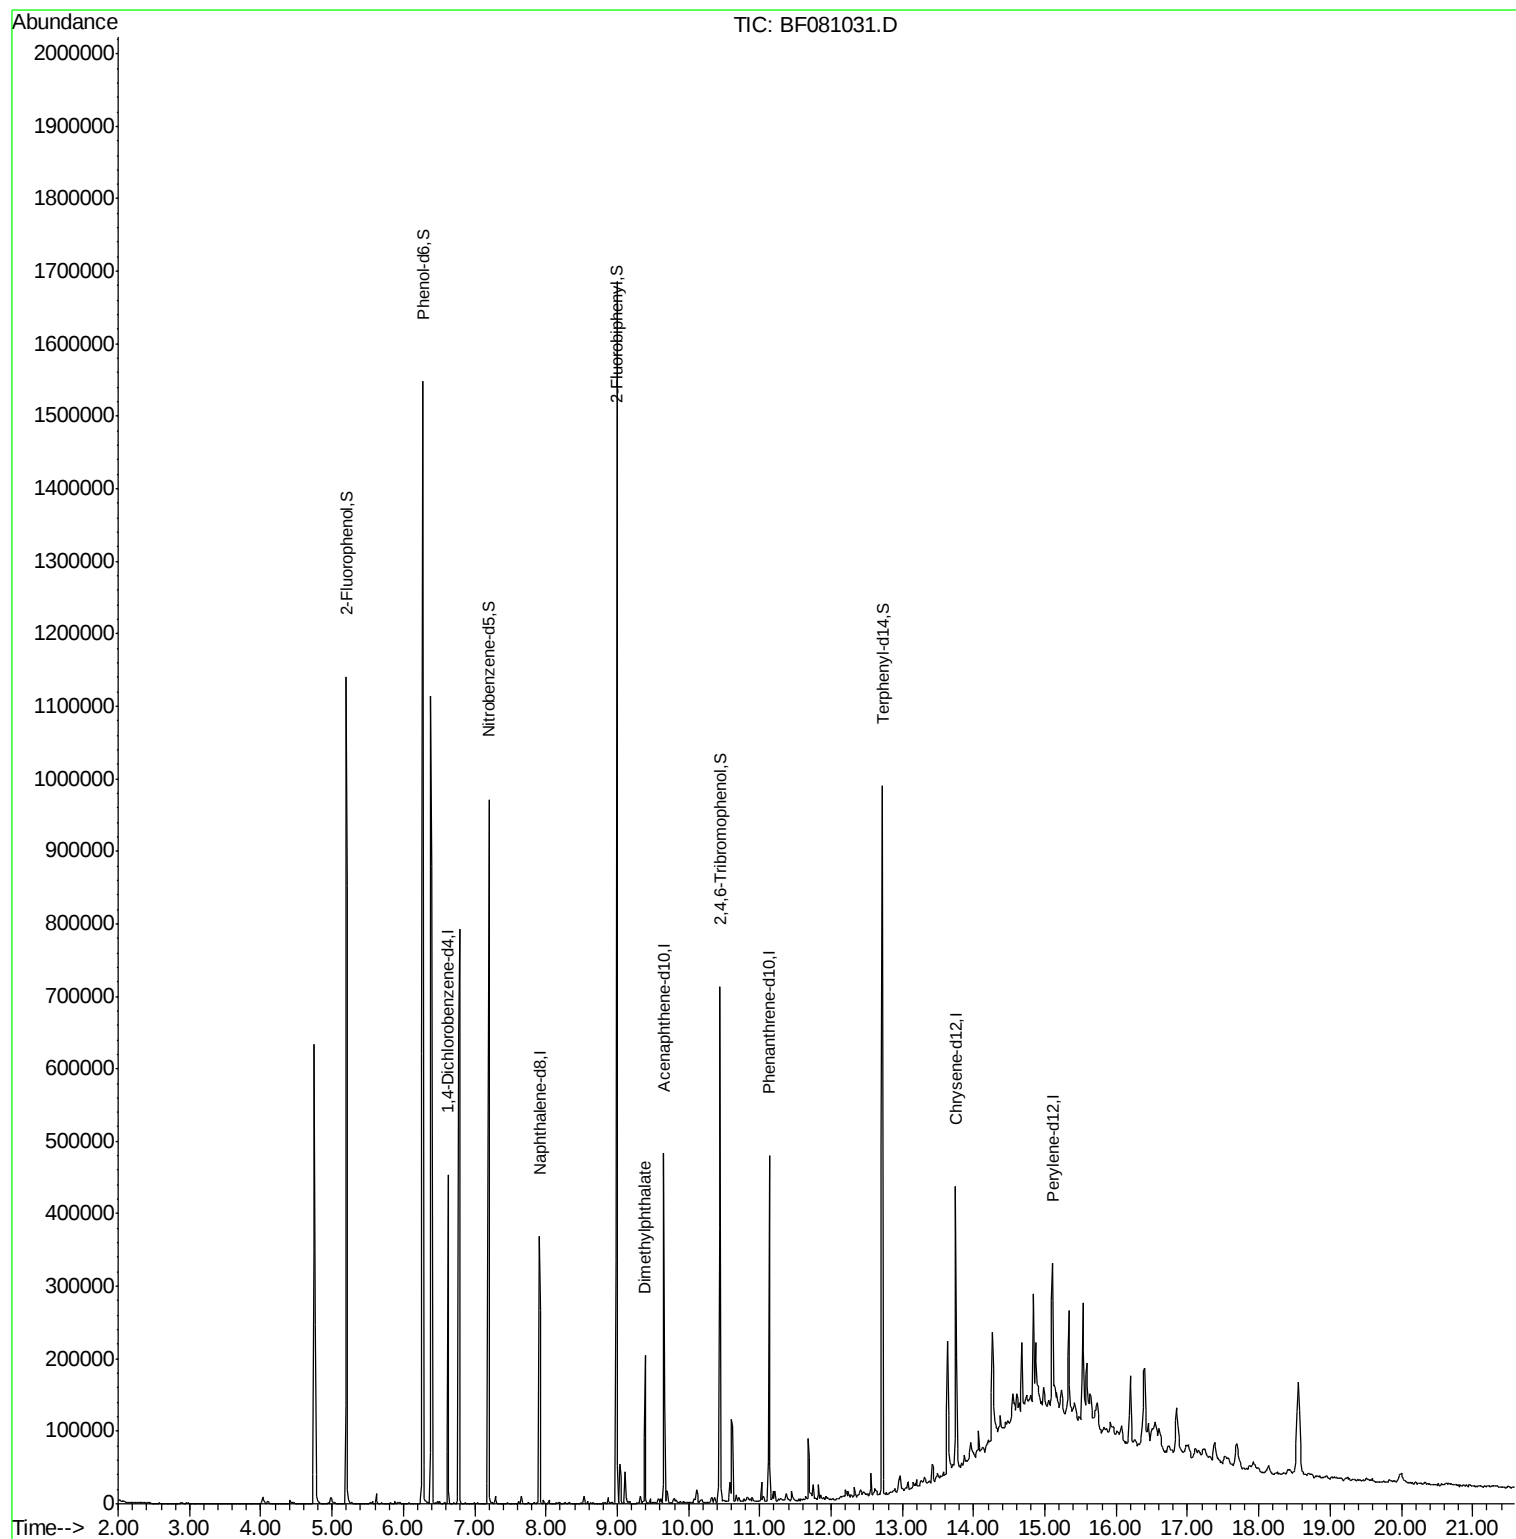

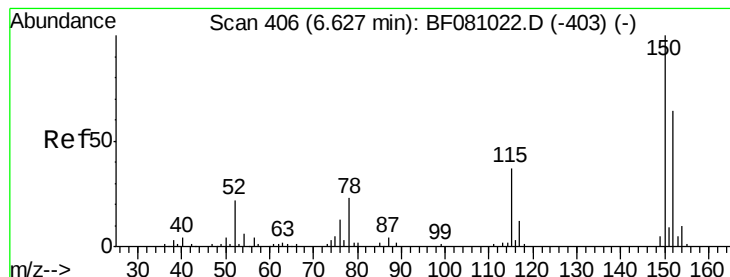

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.63 min Scan# 406

Delta R.T. 0.00 min

Lab File: BF081031.D

Acq: 18 Aug 2015 5:51

Instrument :

BNA_F

ClientSampled :

2A(0-2)-4


Tgt Ion:152 Resp: 59825

Ion Ratio Lower Upper

152 100

150 154.4 123.8 185.6




115 60.6 52.1 78.1

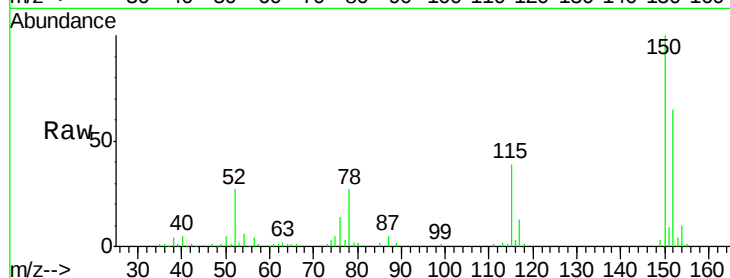

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

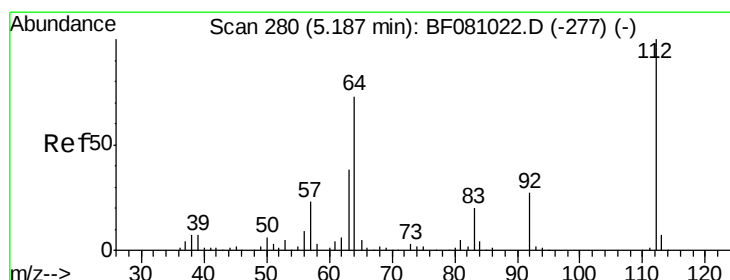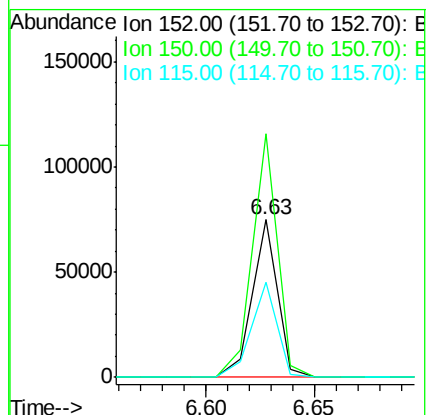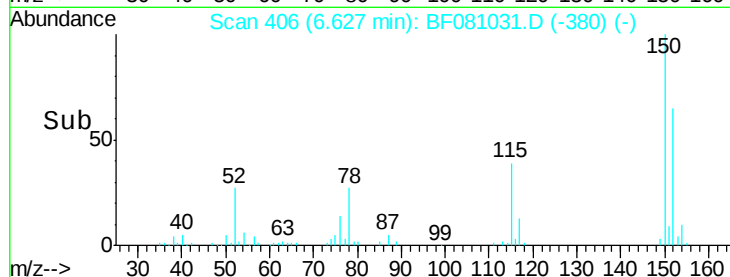

#5

2-Fluorophenol

Concen: 96.36 ng

RT: 5.20 min Scan# 281

Delta R.T. 0.01 min

Lab File: BF081031.D

Acq: 18 Aug 2015 5:51


Tgt Ion:112 Resp: 383263

Ion Ratio Lower Upper

112 100

64 81.1 66.9 100.3



63 43.2 38.1 57.1

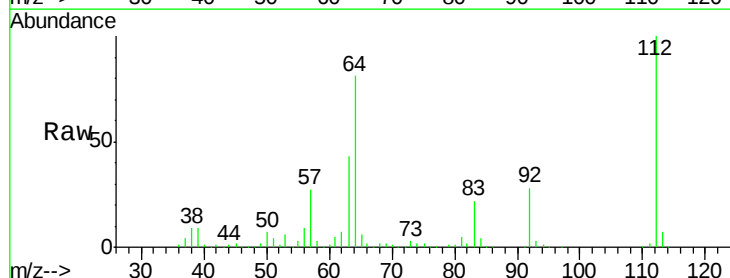


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

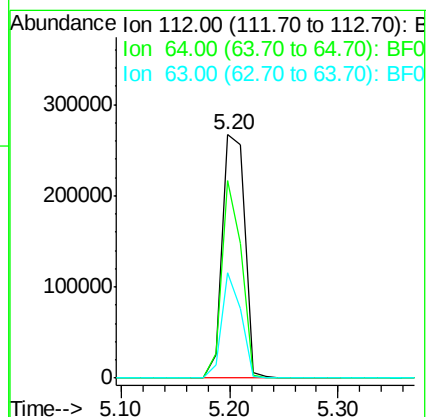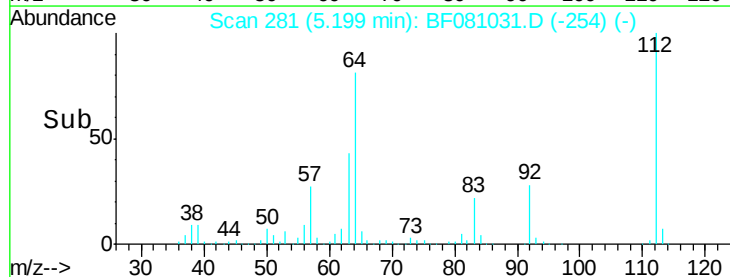

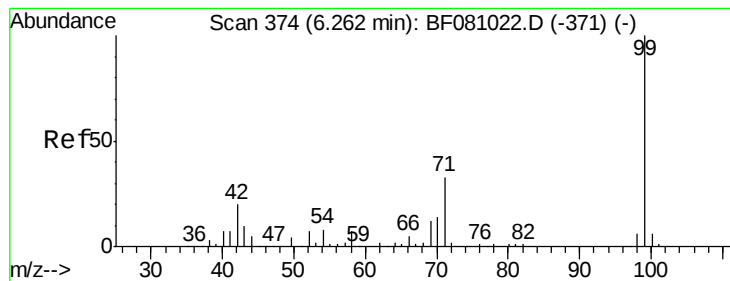

#7

Phenol-d6

Concen: 97.58 ng

RT: 6.27 min Scan# 375

Delta R.T. 0.01 min

Lab File: BF081031.D

Acq: 18 Aug 2015 5:51

Instrument :

BNA_F

ClientSampleId :

2A(0-2)-4


Tgt Ion: 99 Resp: 506413

Ion Ratio Lower Upper

99 100

42 23.3 19.6 29.4




71 36.2 31.2 46.8

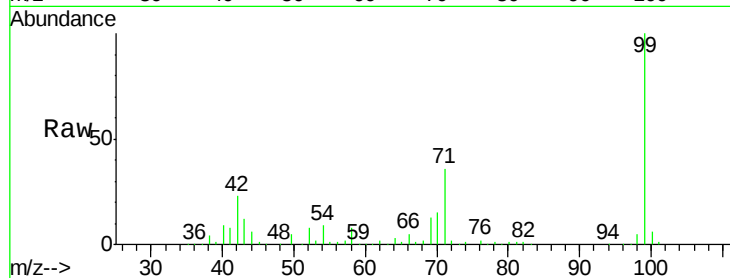

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

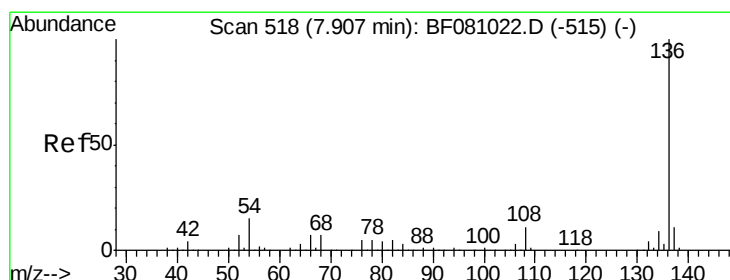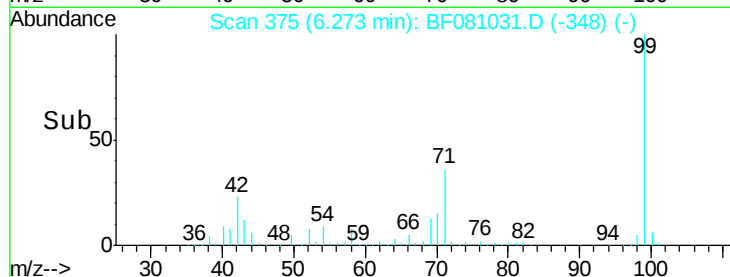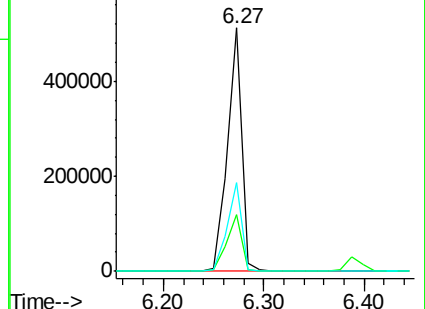

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.91 min Scan# 518

Delta R.T. 0.00 min

Lab File: BF081031.D

Acq: 18 Aug 2015 5:51

Tgt Ion: 136 Resp: 208351


Ion Ratio Lower Upper

136 100

137 11.1 8.2 12.2

54 15.1 7.7 11.5#

68 7.5 3.4 5.2#


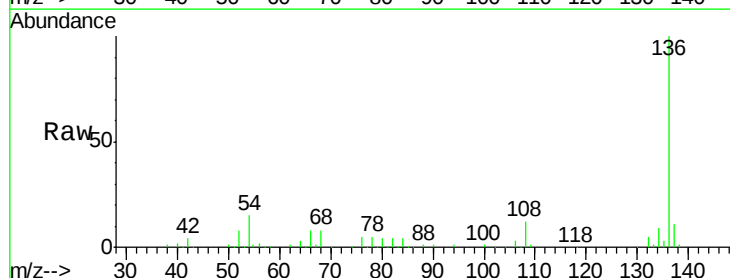



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

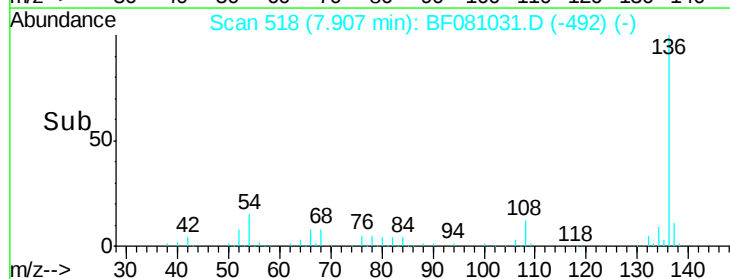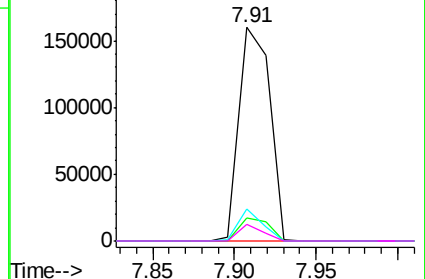


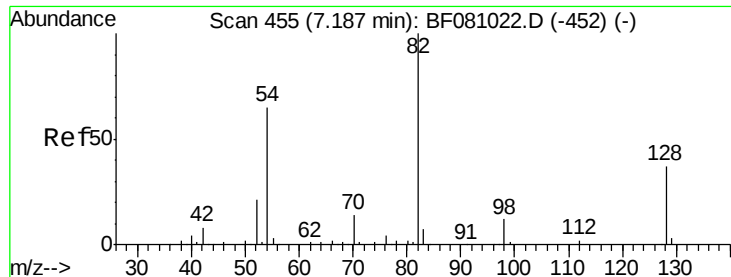




#23
 Nitrobenzene-d5
 Concen: 76.53 ng
 RT: 7.20 min Scan# 456
 Delta R.T. 0.01 min
 Lab File: BF081031.D
 Acq: 18 Aug 2015 5:51

Instrument :
 BNA_F
 ClientSampleId :
 2A(0-2)-4

Tgt Ion: 82 Resp: 349042
 Ion Ratio Lower Upper
 82 100
 128 43.4 28.6 42.8#
 54 58.3 55.1 82.7

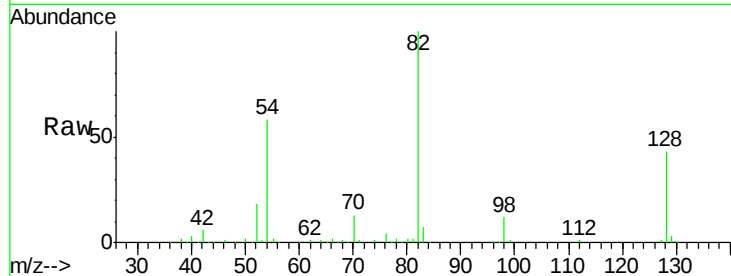


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

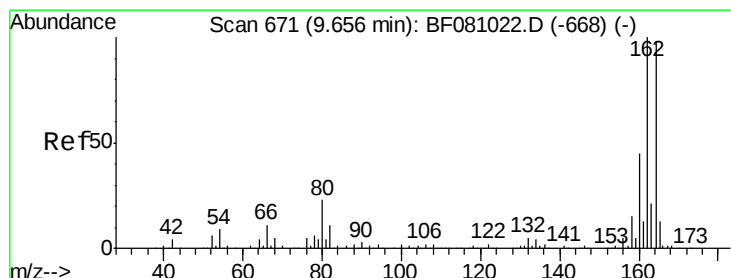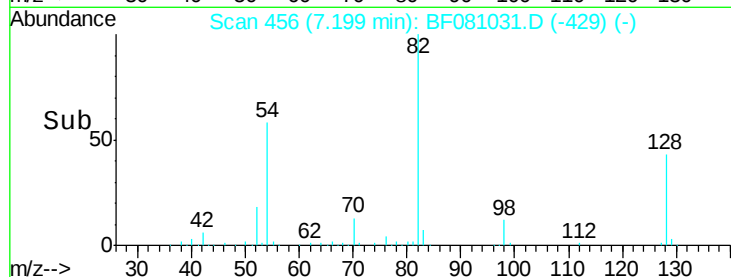
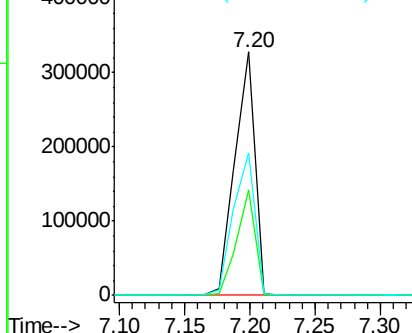



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.66 min Scan# 671
 Delta R.T. 0.00 min
 Lab File: BF081031.D
 Acq: 18 Aug 2015 5:51

Tgt Ion: 164 Resp: 90694
 Ion Ratio Lower Upper
 164 100
 162 102.4 83.8 125.8
 160 46.5 39.8 59.8

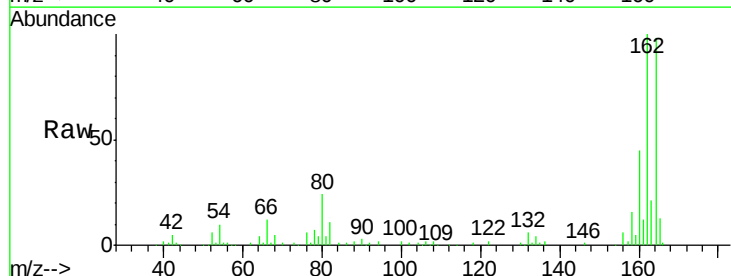

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

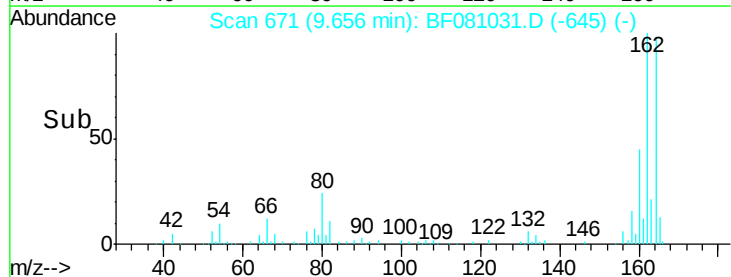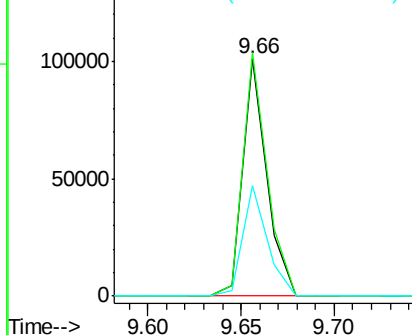


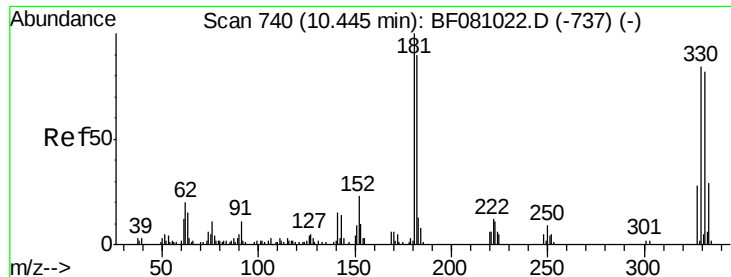




#41
 2,4,6-Tribromophenol
 Concen: 92.95 ng
 RT: 10.44 min Scan# 740
 Delta R.T. 0.00 min
 Lab File: BF081031.D
 Acq: 18 Aug 2015 5:51

Instrument :
 BNA_F
 ClientSampleId :
 2A(0-2)-4

Tgt Ion:330 Resp: 73071
 Ion Ratio Lower Upper
 330 100
 332 92.9 77.3 115.9
 141 51.0 44.9 67.3

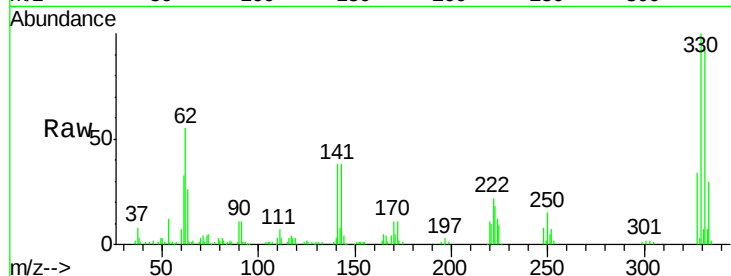


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

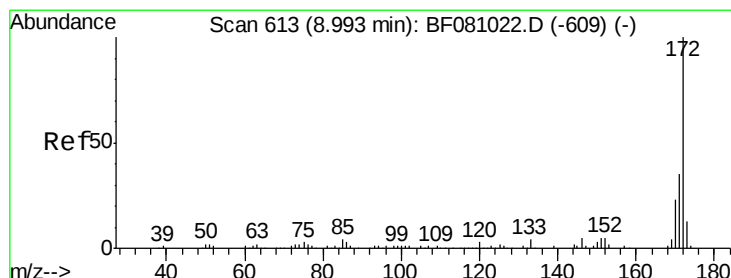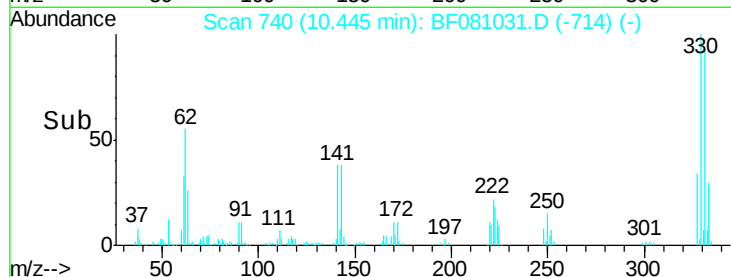
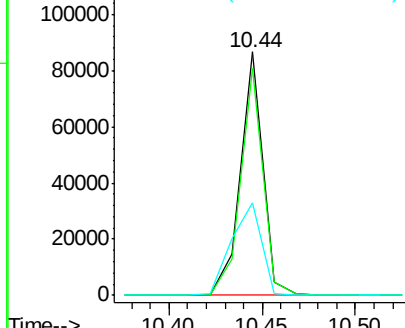



#44
 2-Fluorobiphenyl
 Concen: 66.23 ng
 RT: 8.99 min Scan# 613
 Delta R.T. 0.00 min
 Lab File: BF081031.D
 Acq: 18 Aug 2015 5:51

Tgt Ion:172 Resp: 458416
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.9 43.3
 170 24.6 19.4 29.2

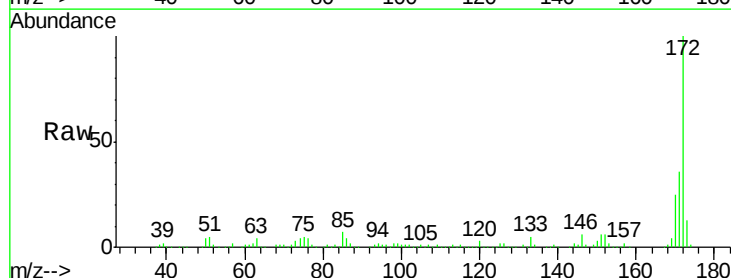

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

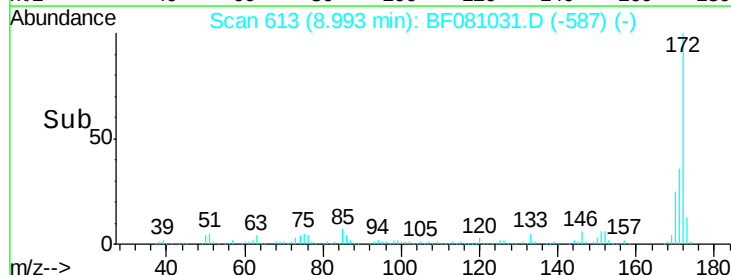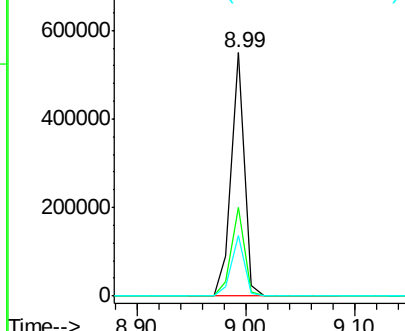


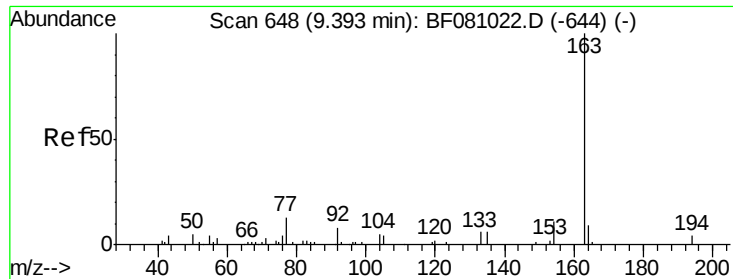




#49
Dimethylphthalate
Concen: 12.18 ng
RT: 9.39 min Scan# 648
Delta R.T. 0.00 min
Lab File: BF081031.D
Acq: 18 Aug 2015 5:51

Instrument :
BNA_F
ClientSampleId :
2A(0-2)-4

Tgt Ion:163 Resp: 91011
Ion Ratio Lower Upper
163 100
194 3.4 2.5 3.7
164 9.7 8.1 12.1

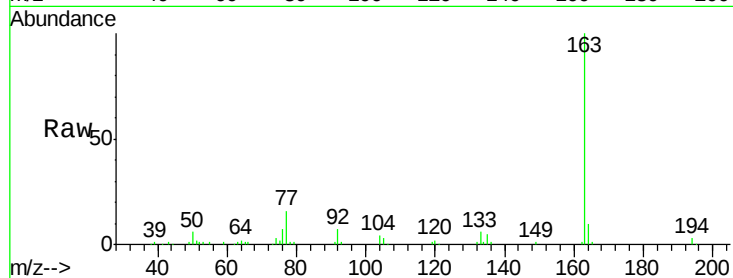


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

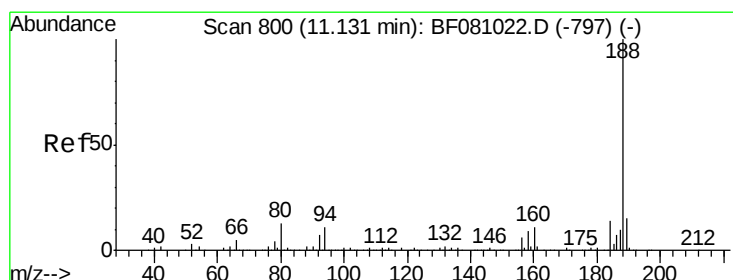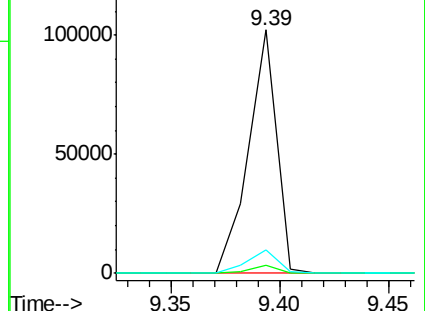
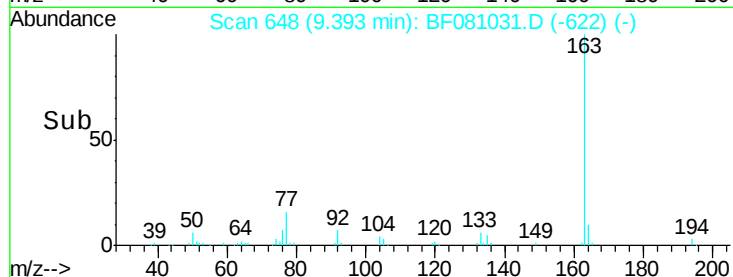



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.13 min Scan# 800
Delta R.T. 0.00 min
Lab File: BF081031.D
Acq: 18 Aug 2015 5:51

Tgt Ion:188 Resp: 157155
Ion Ratio Lower Upper
188 100
94 9.9 8.2 12.2
80 10.3 9.5 14.3

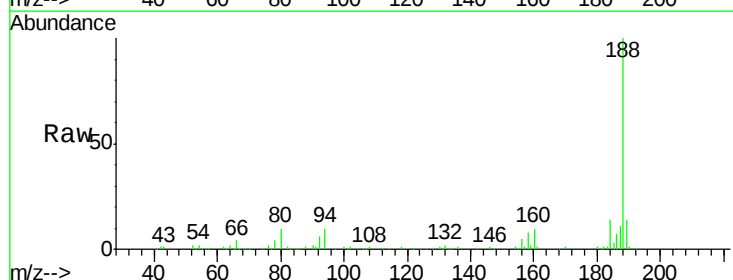

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

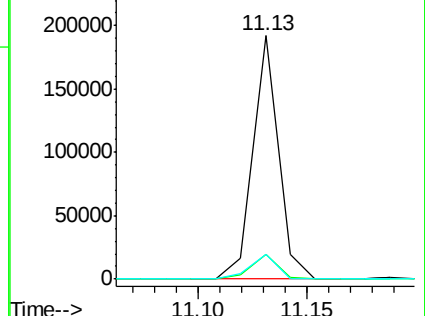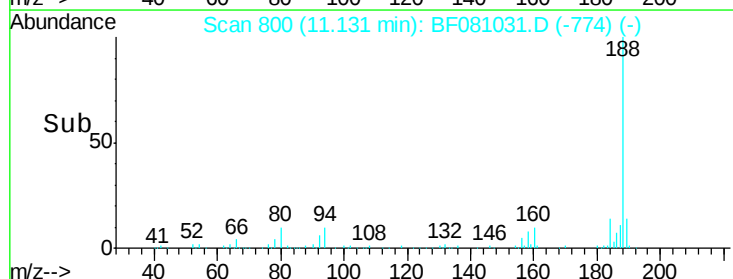

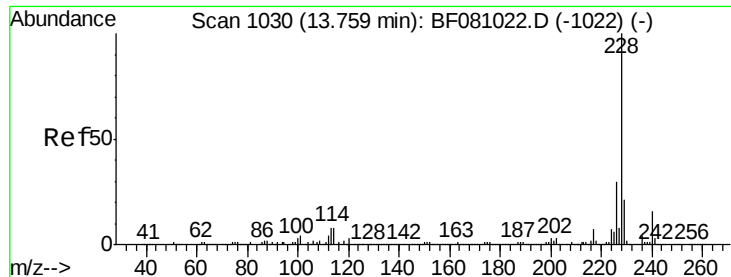

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.75 min Scan# 1029

Delta R.T. 0.00 min

Lab File: BF081031.D

Acq: 18 Aug 2015 5:51

Instrument :

BNA_F

ClientSampleId :

2A(0-2)-4


Tgt Ion:240 Resp: 125210

Ion Ratio Lower Upper

240 100

120 14.1 5.6 8.4#




236 25.2 20.6 30.8

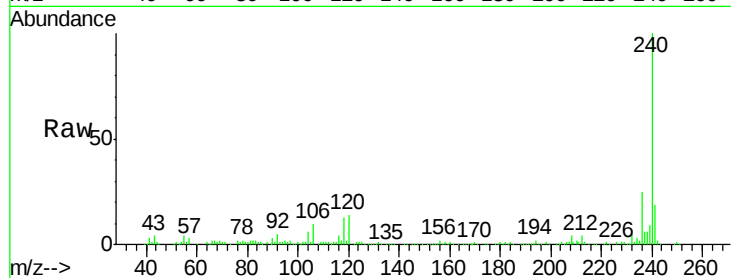

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

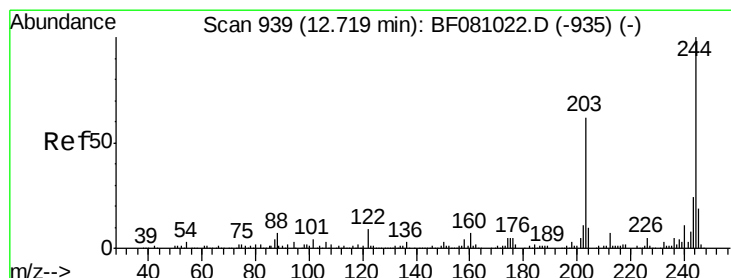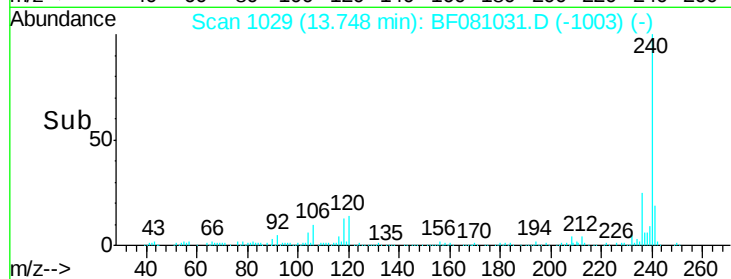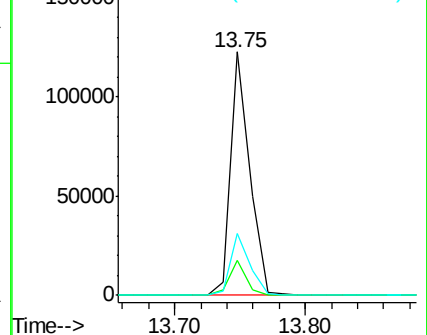

#78

Terphenyl-d14

Concen: 55.02 ng

RT: 12.72 min Scan# 939

Delta R.T. 0.01 min

Lab File: BF081031.D

Acq: 18 Aug 2015 5:51


Tgt Ion:244 Resp: 321360

Ion Ratio Lower Upper

244 100

212 7.5 5.8 8.8



122 9.7 8.2 12.4

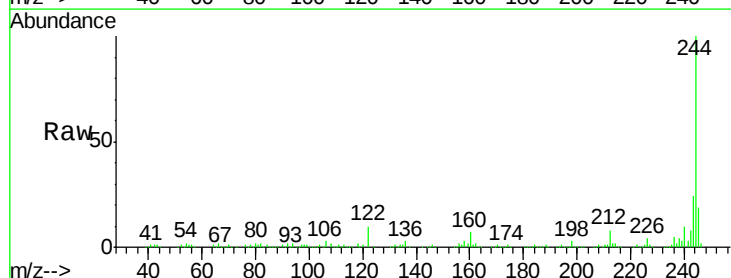


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

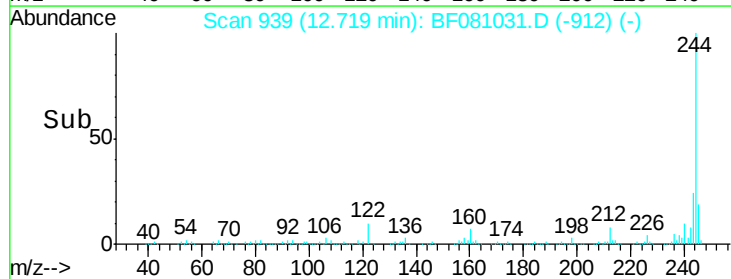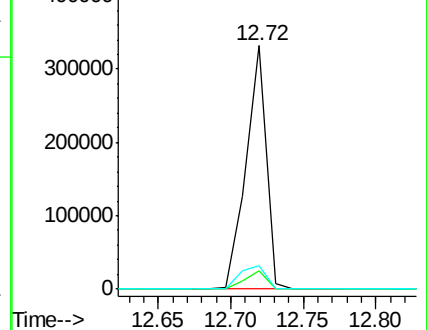

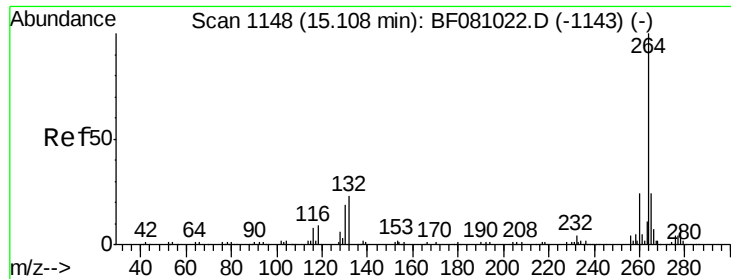

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.11 min Scan# 1148
Delta R.T. 0.01 min
Lab File: BF081031.D
Acq: 18 Aug 2015 5:51

Instrument :
BNA_F
ClientSampleId :
2A(0-2)-4

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.6	29.4
265	21.8	17.5	26.3

