


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081715\
 Data File : BF080999.D
 Acq On : 17 Aug 2015 11:48
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 17:57:25 2015

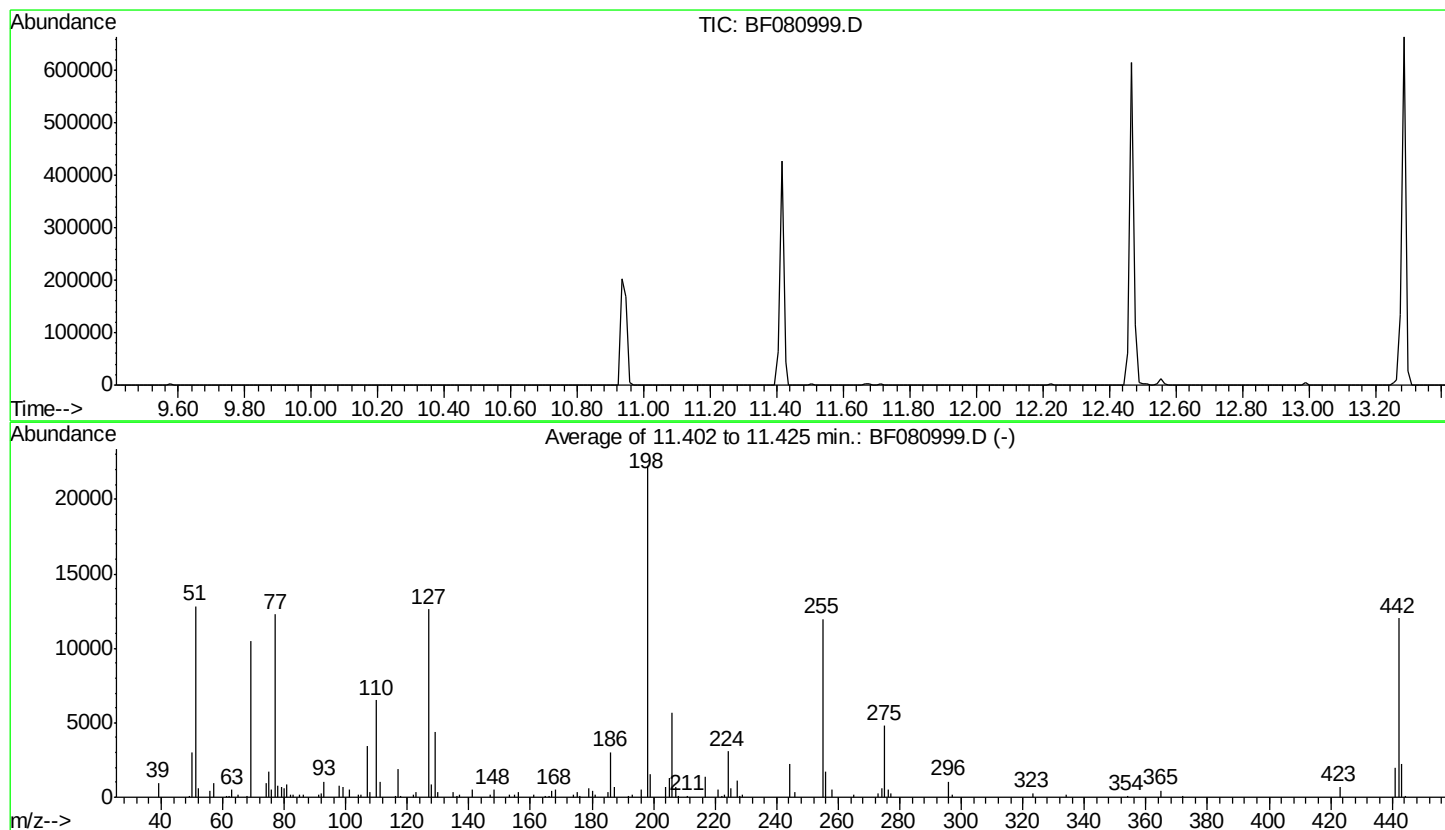

AutoFind: Scans 815, 816, 817; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	12849	PASS
68	69	0.00	2	1.1	110	PASS
69	198	0.00	100	47.0	10475	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	12620	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22267	PASS
199	198	5	9	6.9	1545	PASS
275	198	10	60	21.4	4775	PASS
365	198	1	100	2.0	437	PASS
441	442	0.01	24	16.3	1961	PASS
442	198	50	100	53.9	12011	PASS
443	442	15	24	18.8	2263	PASS