


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081715\
 Data File : BF081020.D
 Acq On : 18 Aug 2015 00:04
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 17:57:25 2015

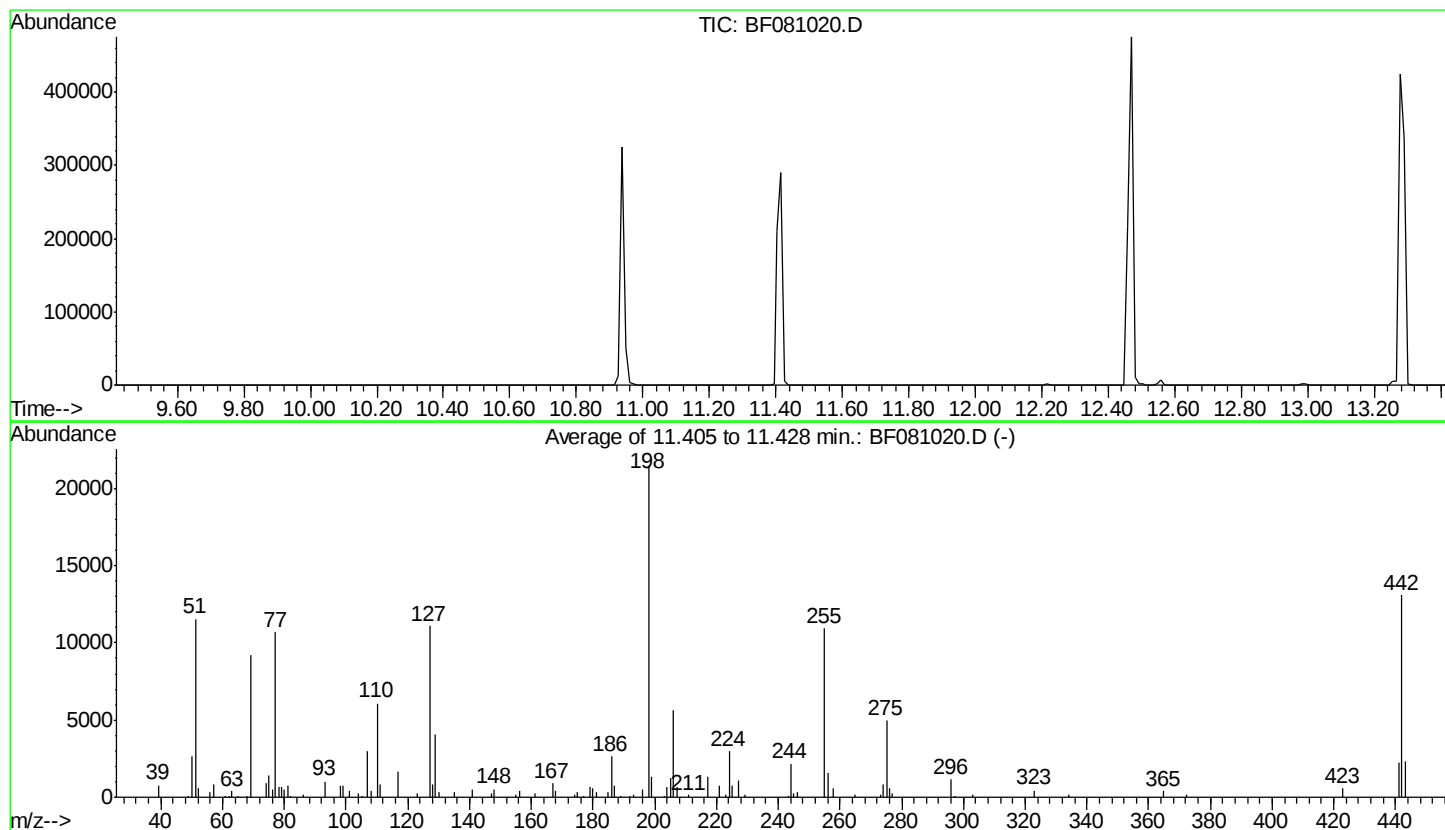

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	11546	PASS
68	69	0.00	2	1.3	123	PASS
69	198	0.00	100	42.7	9170	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	11101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21471	PASS
199	198	5	9	6.3	1356	PASS
275	198	10	60	23.0	4941	PASS
365	198	1	100	1.8	378	PASS
441	442	0.01	24	17.0	2222	PASS
442	198	50	100	60.8	13058	PASS
443	442	15	24	17.5	2285	PASS