


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081716\
Data File : BF089759.D
Acq On : 17 Aug 2016 13:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 16 19:45:04 2016

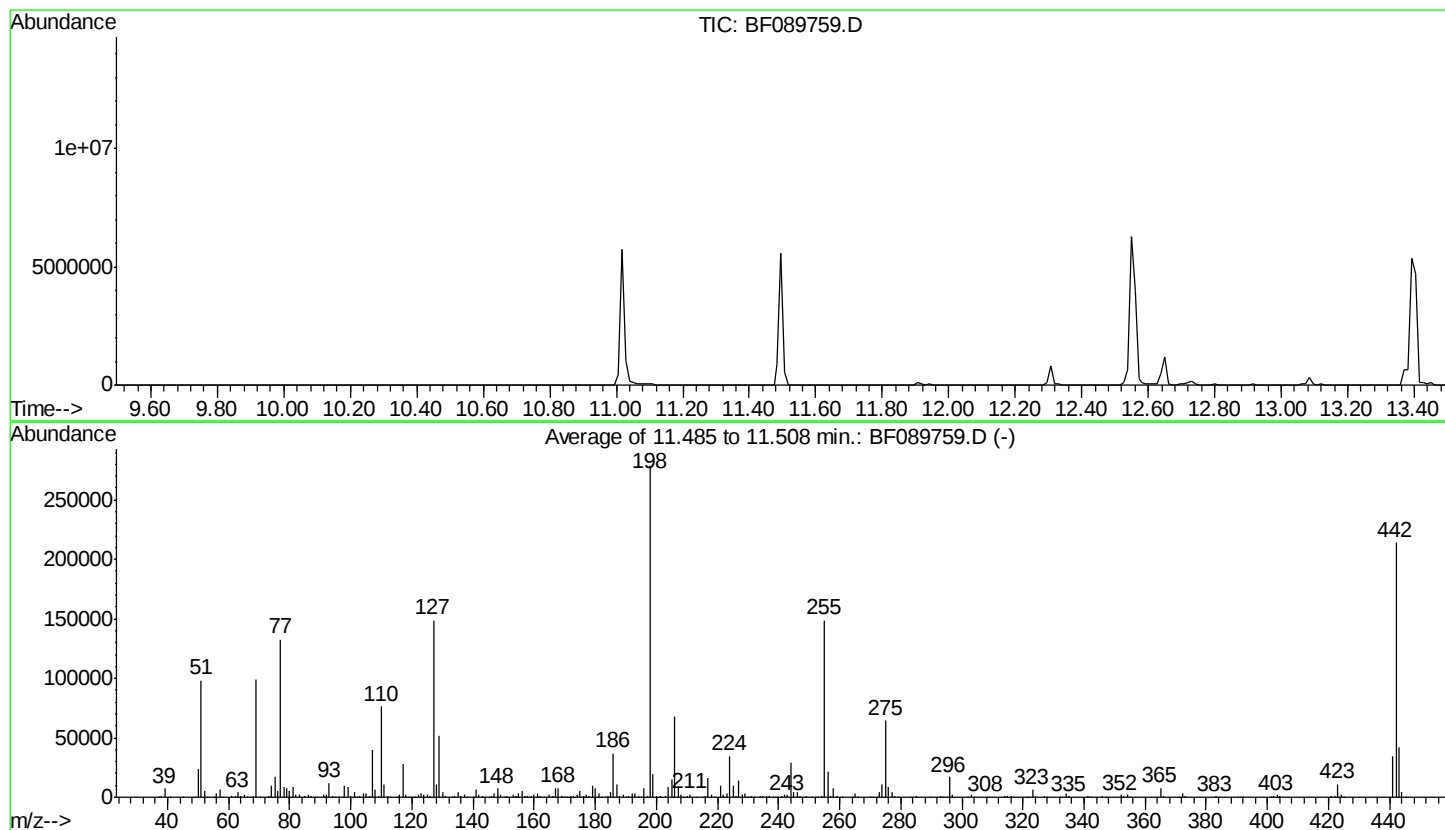

AutoFind: Scans 866, 867, 868; Background Corrected with Scan 862

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	97987	PASS
68	69	0.00	2	1.5	1485	PASS
69	198	0.00	100	35.6	99345	PASS
70	69	0.00	2	0.5	494	PASS
127	198	10	80	53.4	149007	PASS
197	198	0.00	2	0.4	1247	PASS
198	198	100	100	100.0	278800	PASS
199	198	5	9	6.8	18953	PASS
275	198	10	60	23.0	64181	PASS
365	198	1	100	2.8	7765	PASS
441	442	0.01	24	16.3	34778	PASS
442	198	50	100	76.7	213925	PASS
443	442	15	24	19.4	41582	PASS