
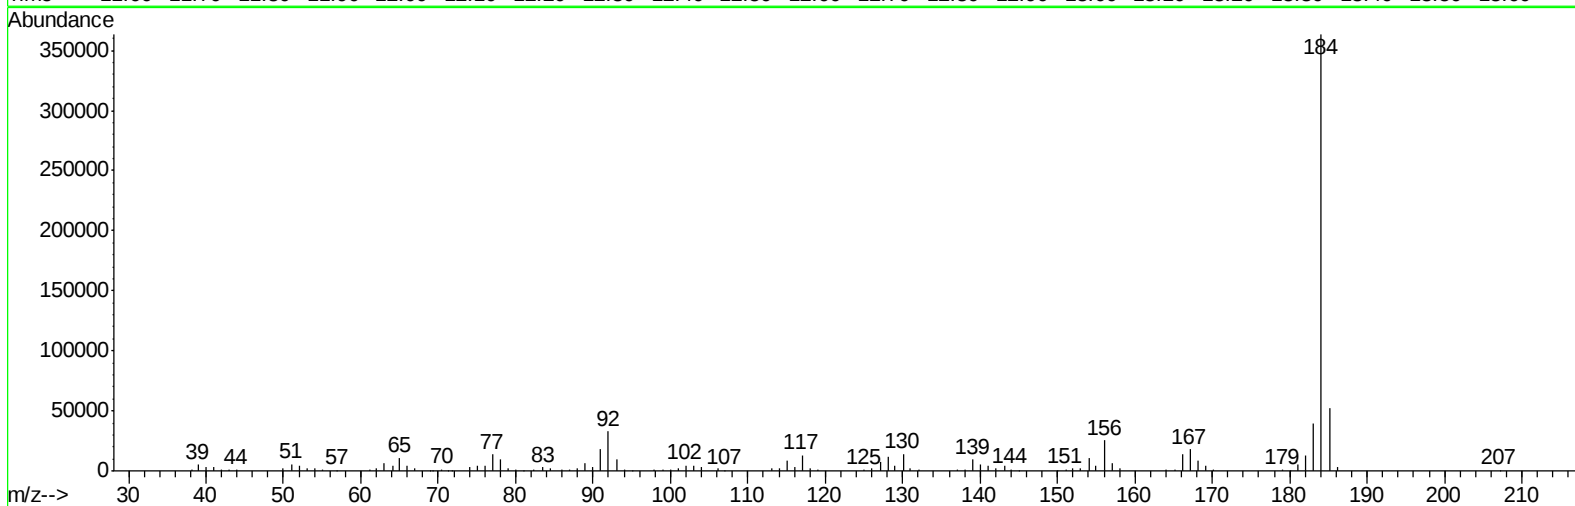


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081717\
Data File : BF097811.D
Acq On : 18 Aug 2017 3:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 07:46:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

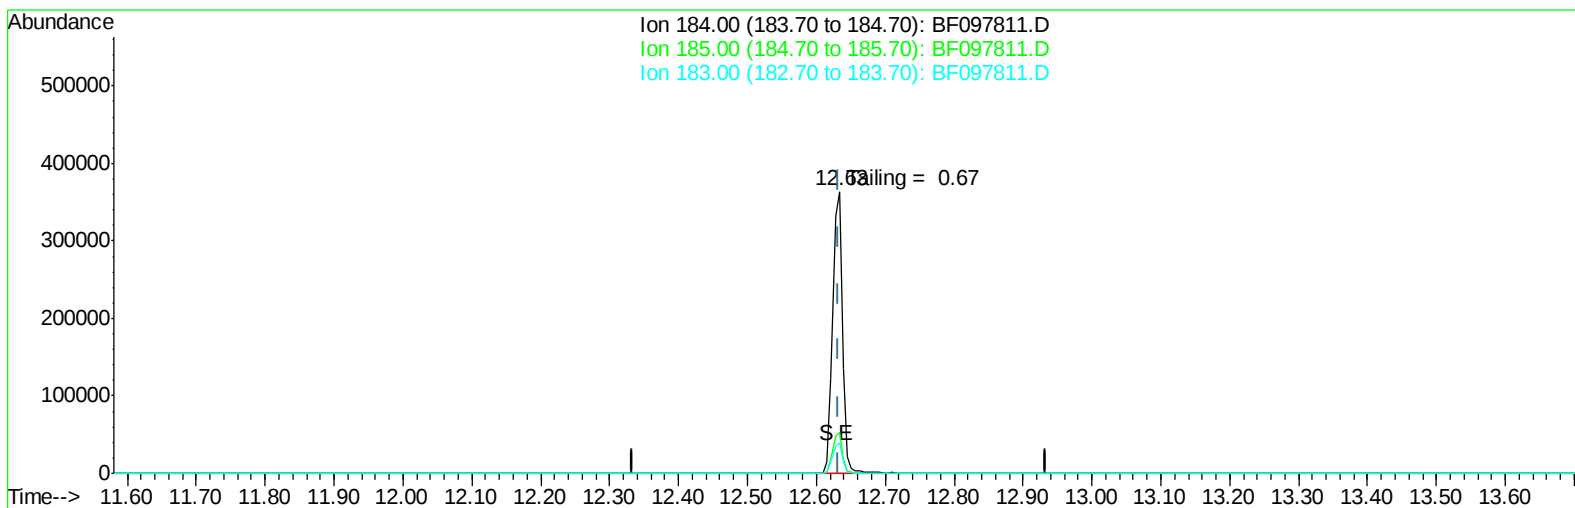

TIC: BF097811.D

(76) Benzidine



12.633min (+0.000) 0.00ng

response 358185

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.35#
183.00	12.20	11.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081717\
Data File : BF097811.D
Acq On : 18 Aug 2017 3:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 07:46:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

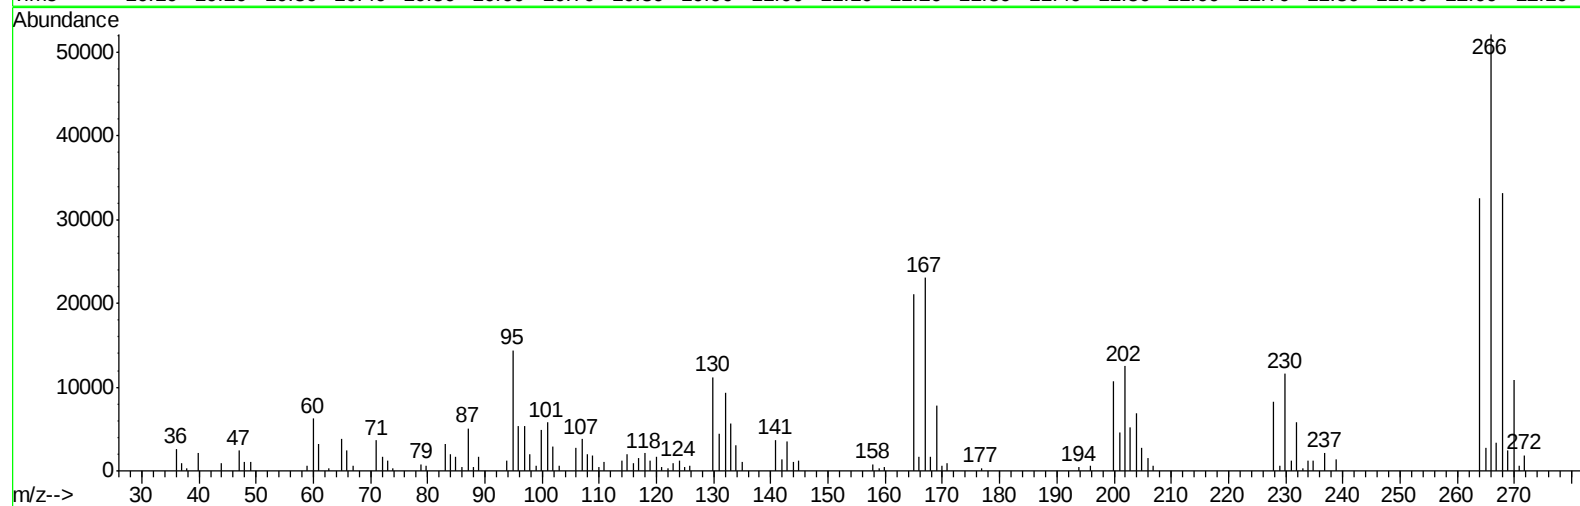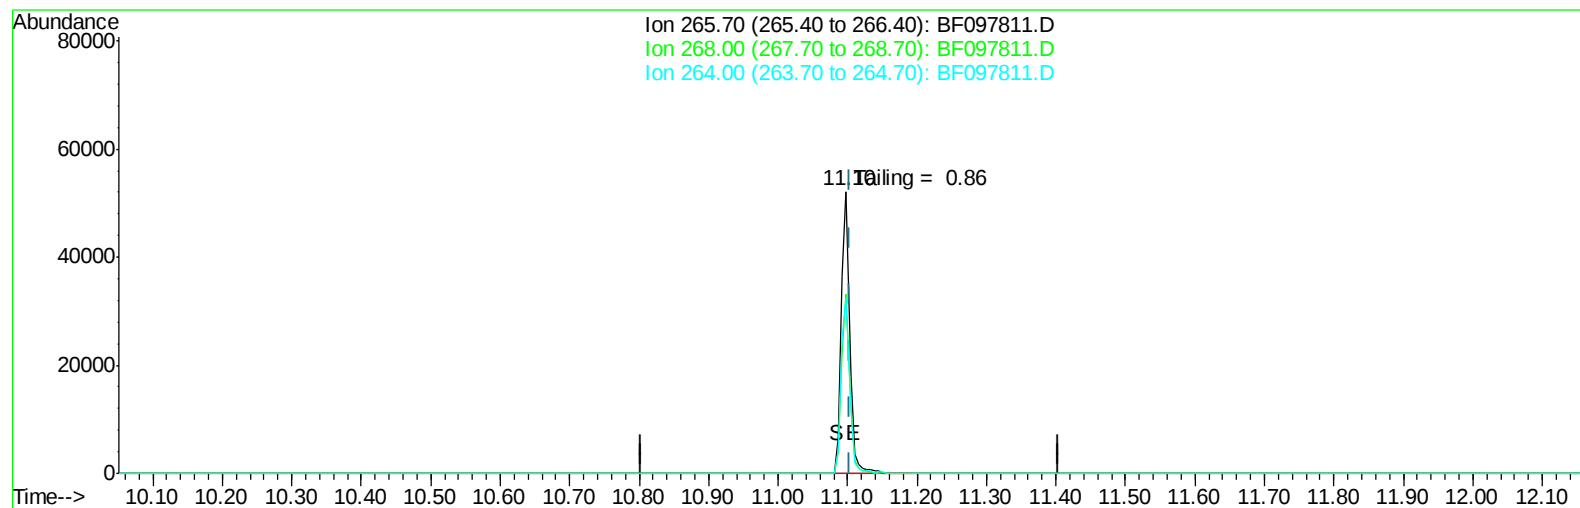

TIC: BF097811.D

(69) Pentachlorophenol (C)

11.098min (-0.006) 57604.65ng

response 43015

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.63
264.00	64.60	62.48
0.00	0.00	0.00