

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081717\
 Data File : BF097818.D
 Acq On : 18 Aug 2017 6:56
 Operator : SJ/JU
 Sample : I4794-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CEMENT-BLOCK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	184	186	198	rBV	65889	127577	3.64%	0.338%
2	4.975	487	491	499	rVB	306858	388040	11.06%	1.028%
3	5.387	556	561	564	rBV	2931467	2895678	82.55%	7.674%
4	5.716	614	617	626	rVB	87986	78287	2.23%	0.207%
5	5.934	651	654	662	rVB	41742	52151	1.49%	0.138%
6	6.010	662	667	676	rBV	181599	236491	6.74%	0.627%
7	6.310	714	718	723	rBV	105893	128389	3.66%	0.340%
8	6.410	728	735	746	rVB	2880690	3183362	90.75%	8.436%
9	6.545	753	758	761	rBV	3038285	2844414	81.08%	7.538%
10	6.587	761	765	766	rVV	76872	65125	1.86%	0.173%
11	6.616	766	770	773	rVB	1157143	1103151	31.45%	2.923%
12	6.704	782	785	789	rBV	249992	198972	5.67%	0.527%
13	6.775	793	797	801	rBV	1092775	896342	25.55%	2.375%
14	6.869	810	813	816	rVB	48570	38404	1.09%	0.102%
15	6.934	816	824	827	rBV	2692593	2441686	69.60%	6.470%
16	7.339	888	893	896	rBV	1992992	1809569	51.58%	4.795%
17	7.463	909	914	917	rBV	102799	118580	3.38%	0.314%
18	7.775	960	967	970	rBV	1477204	2042535	58.23%	5.413%
19	7.804	970	972	977	rVB	99718	90980	2.59%	0.241%
20	7.981	995	1002	1004	rBV	2822755	3507988	100.00%	9.296%
21	8.057	1011	1015	1019	rBV	1108723	957276	27.29%	2.537%
22	8.210	1039	1041	1046	rVB	61129	52637	1.50%	0.139%
23	8.292	1051	1055	1056	rBV2	32024	35137	1.00%	0.093%
24	8.310	1056	1058	1067	rVB	33889	35360	1.01%	0.094%
25	8.404	1067	1074	1079	rBV	97870	110373	3.15%	0.292%
26	8.457	1079	1083	1086	rBV	80151	80660	2.30%	0.214%
27	8.798	1135	1141	1144	rBV	78581	82622	2.36%	0.219%
28	9.010	1173	1177	1181	rBV	983531	833835	23.77%	2.210%
29	9.139	1193	1199	1202	rBV2	2862823	3350897	95.52%	8.880%
30	9.228	1211	1214	1216	rBV3	39355	35415	1.01%	0.094%
31	9.257	1216	1219	1227	rVB2	145042	160656	4.58%	0.426%
32	9.410	1242	1245	1249	rVB	63929	48679	1.39%	0.129%
33	9.451	1249	1252	1256	rBV	81869	64564	1.84%	0.171%
34	9.528	1262	1265	1269	rVB	298688	245233	6.99%	0.650%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081717\
 Data File : BF097818.D
 Acq On : 18 Aug 2017 6:56
 Operator : SJ/JU
 Sample : I4794-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CEMENT-BLOCK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.569	1269	1272	1278	rVV2	170989	147183	4.20%	0.390%
36	9.622	1278	1281	1287	rVB	160978	138228	3.94%	0.366%
37	9.692	1289	1293	1300	rBV	293735	271486	7.74%	0.719%
38	9.810	1306	1313	1318	rBV	908415	868872	24.77%	2.303%
39	9.857	1318	1321	1324	rVB	77901	69129	1.97%	0.183%
40	9.969	1336	1340	1345	rBV	45518	43690	1.25%	0.116%
41	10.022	1345	1349	1351	rBV	180325	165179	4.71%	0.438%
42	10.222	1380	1383	1386	rBV2	230427	230167	6.56%	0.610%
43	10.439	1417	1420	1423	rBV2	34866	38705	1.10%	0.103%
44	10.510	1429	1432	1437	rVB2	76100	66753	1.90%	0.177%
45	10.598	1442	1447	1450	rBV	1373224	1229291	35.04%	3.258%
46	10.622	1450	1451	1456	rVB	75152	55909	1.59%	0.148%
47	10.722	1465	1468	1477	rVB	68142	76790	2.19%	0.203%
48	10.880	1492	1495	1498	rBV	42677	39356	1.12%	0.104%
49	11.169	1541	1544	1547	rBV2	59571	54559	1.56%	0.145%
50	11.263	1556	1560	1562	rBV	109801	90774	2.59%	0.241%
51	11.292	1562	1565	1569	rVV	783549	687425	19.60%	1.822%
52	11.363	1572	1577	1579	rBV3	44286	49677	1.42%	0.132%
53	11.469	1592	1595	1597	rBV	51458	46723	1.33%	0.124%
54	11.598	1614	1617	1621	rBV	57232	53662	1.53%	0.142%
55	11.633	1621	1623	1631	rVB2	50536	51946	1.48%	0.138%
56	11.863	1659	1662	1665	rBV	216863	165464	4.72%	0.438%
57	12.004	1683	1686	1689	rBV	107681	82314	2.35%	0.218%
58	12.286	1730	1734	1737	rBV	26440	36970	1.05%	0.098%
59	12.392	1749	1752	1755	rBV	222495	178964	5.10%	0.474%
60	12.763	1812	1815	1818	rBV	259761	222594	6.35%	0.590%
61	12.880	1831	1835	1839	rBV	2265553	2128845	60.69%	5.641%
62	13.121	1873	1876	1879	rBV	150256	117060	3.34%	0.310%
63	13.357	1913	1916	1922	rVB	62415	57807	1.65%	0.153%
64	13.463	1931	1934	1937	rVB	66407	54634	1.56%	0.145%
65	13.733	1977	1980	1983	rVB	51070	53136	1.51%	0.141%
66	13.780	1983	1988	1995	rBV3	169245	233939	6.67%	0.620%
67	13.927	2009	2013	2017	rBV	913416	836613	23.85%	2.217%
68	14.415	2093	2096	2100	rVB	45651	44271	1.26%	0.117%
69	14.521	2108	2114	2119	rBV7	26076	46274	1.32%	0.123%
70	14.786	2155	2159	2164	rBV	68551	67555	1.93%	0.179%
71	15.039	2199	2202	2205	rBV	36026	35226	1.00%	0.093%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081717\
Data File : BF097818.D
Acq On : 18 Aug 2017 6:56
Operator : SJ/JU
Sample : I4794-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CEMENT-BLOCK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	15.357	2251	2256	2261	rBV	453924	518066	14.77%	1.373%
73	15.833	2333	2337	2341	rBV2	25707	39514	1.13%	0.105%


Sum of corrected areas: 37735815

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081717\
Data File : BF097818.D
Acq On : 18 Aug 2017 6:56
Operator : SJ/JU
Sample : I4794-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CEMENT-BLOCK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

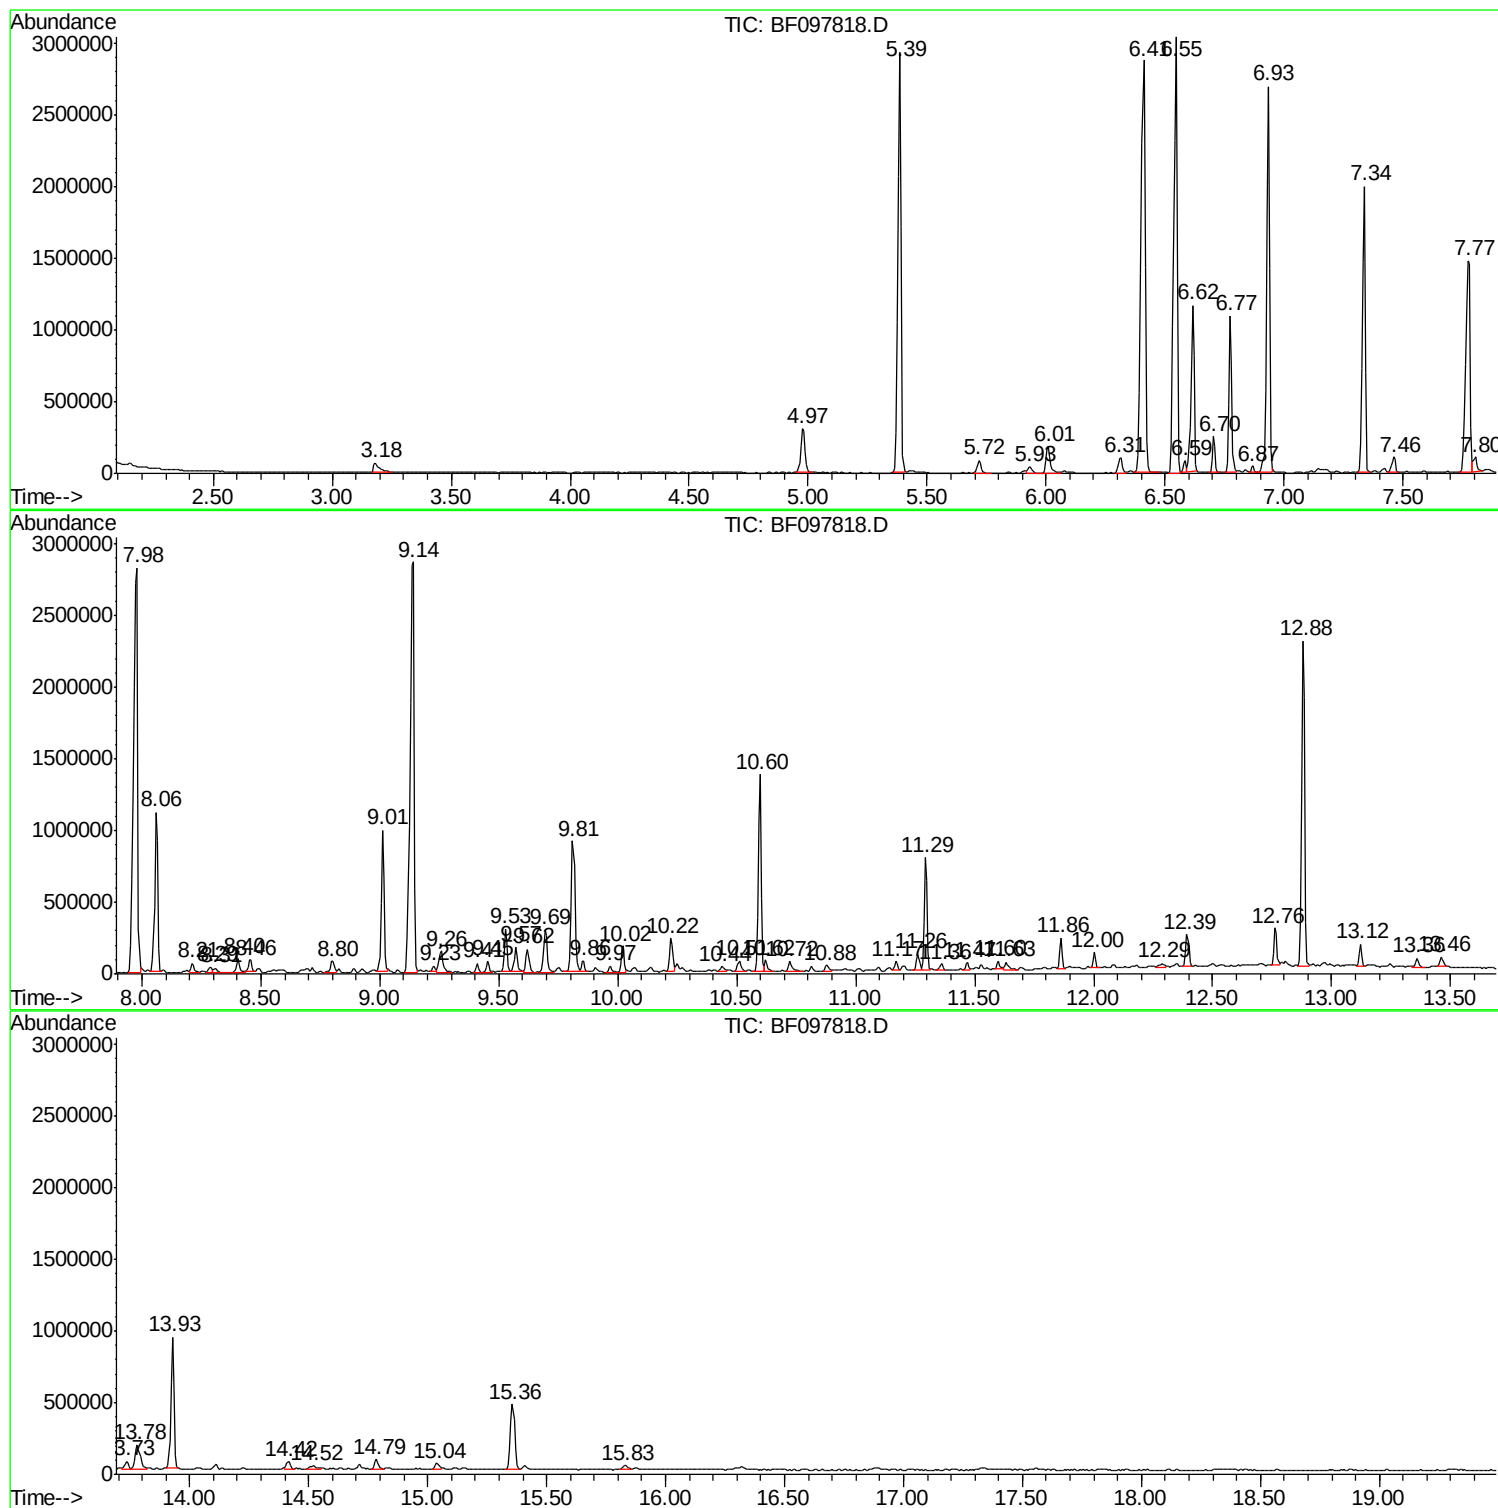

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF081717\
Data_File : BF097818.D
Acq_On : 18_Aug_2017. 6:566
Operator : SJ/JUU
Sample : I4794-011
Misc :
ALS_Vial : 32 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
CEMENT-BLOCK

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
