


Data Path : Z:\HPCHEM1\BNA F\Data\BF081717\
 Data File : BF097785.D
 Acq On : 17 Aug 2017 14:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

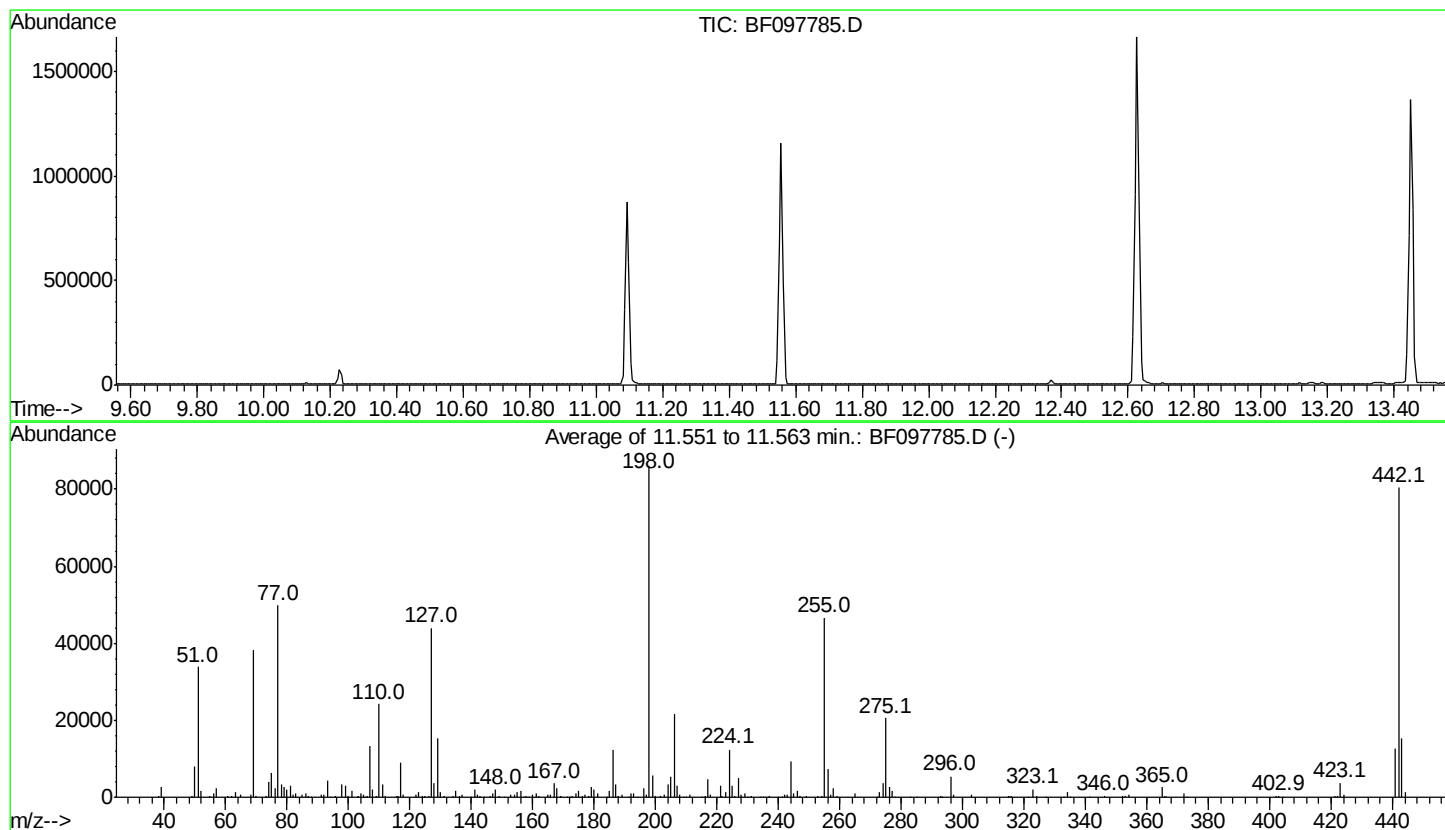

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	33862	PASS
68	69	0.00	2	2.0	748	PASS
69	198	0.00	100	44.5	38325	PASS
70	69	0.00	2	0.6	228	PASS
127	198	10	80	51.2	44064	PASS
197	198	0.00	2	1.0	837	PASS
198	198	100	100	100.0	86138	PASS
199	198	5	9	6.7	5773	PASS
275	198	10	60	23.9	20572	PASS
365	198	1	100	3.1	2643	PASS
441	442	0.01	24	15.6	12504	PASS
442	198	50	100	93.3	80397	PASS
443	442	15	24	19.2	15443	PASS