
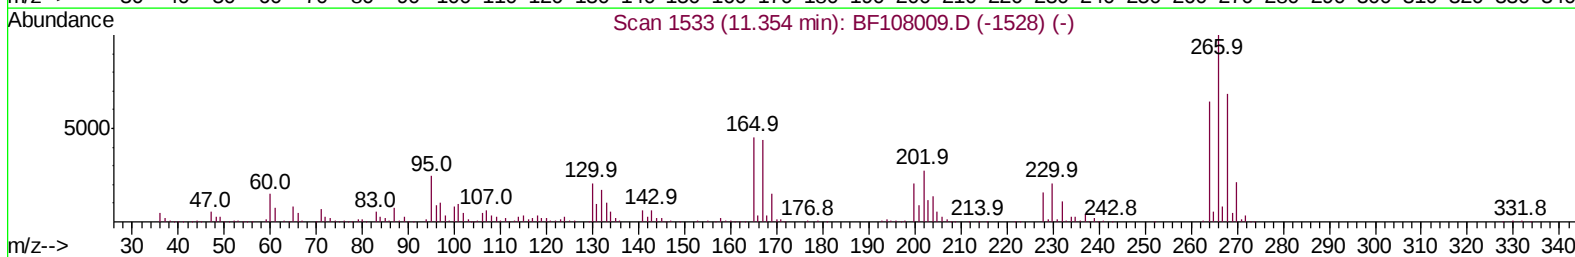
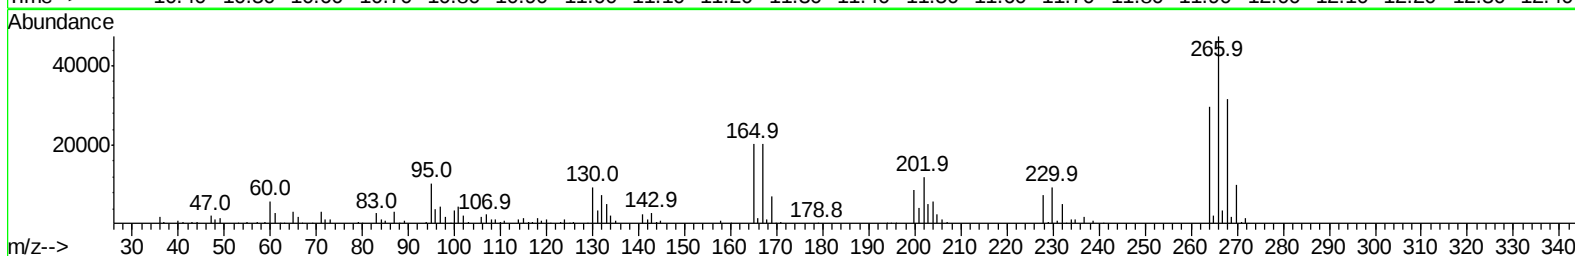


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081718\
Data File : BF108258.D
Acq On : 17 Aug 2018 22:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 03:28:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

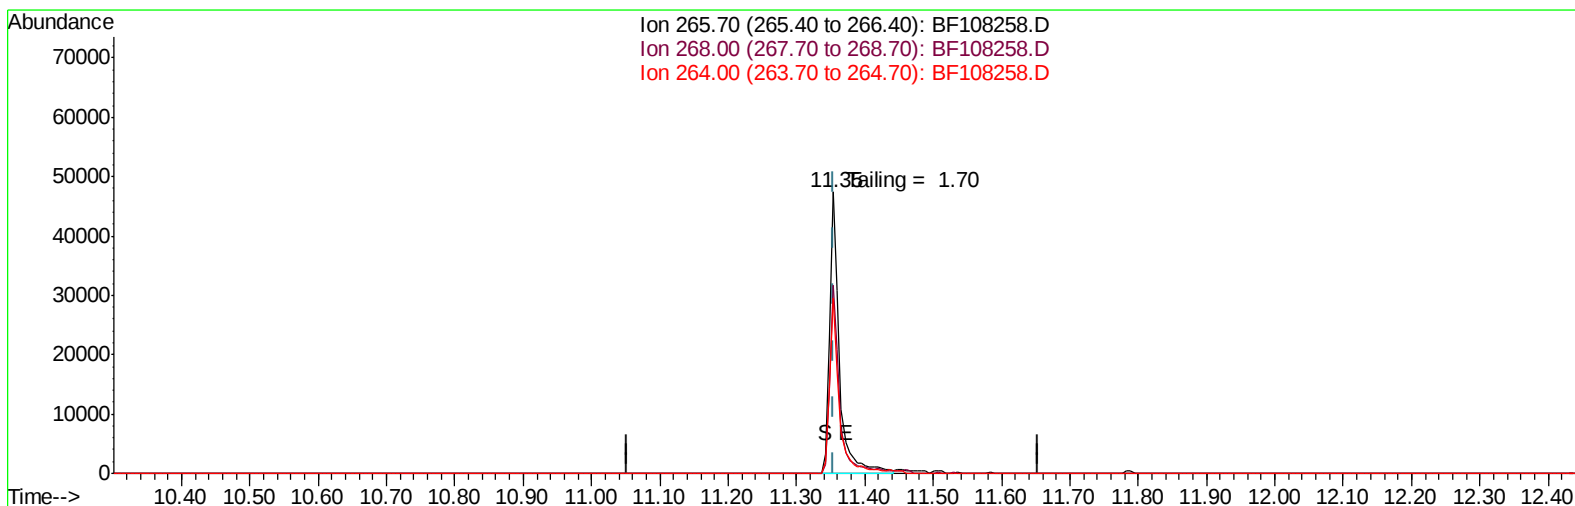

TIC: BF108258.D

(69) Pentachlorophenol (C)




11.354min (0.000) 28780.69ng

response 48199

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.98
264.00	61.90	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081718\
 Data File : BF108258.D
 Acq On : 17 Aug 2018 22:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 03:28:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

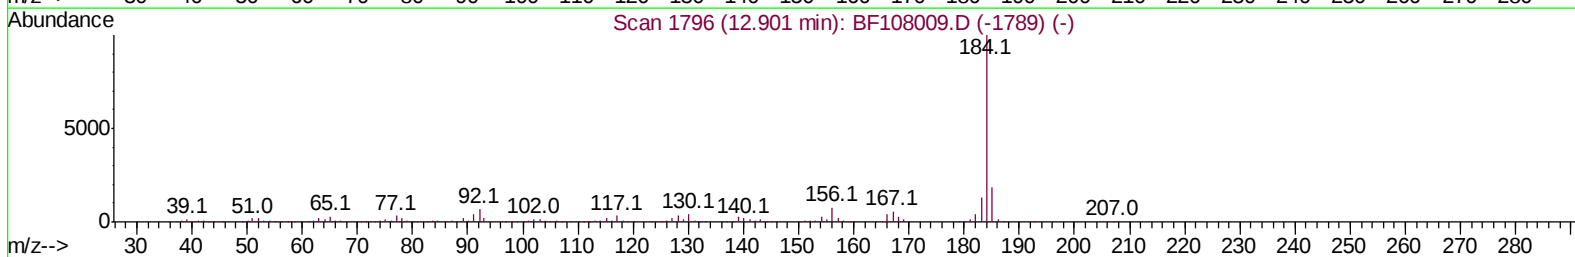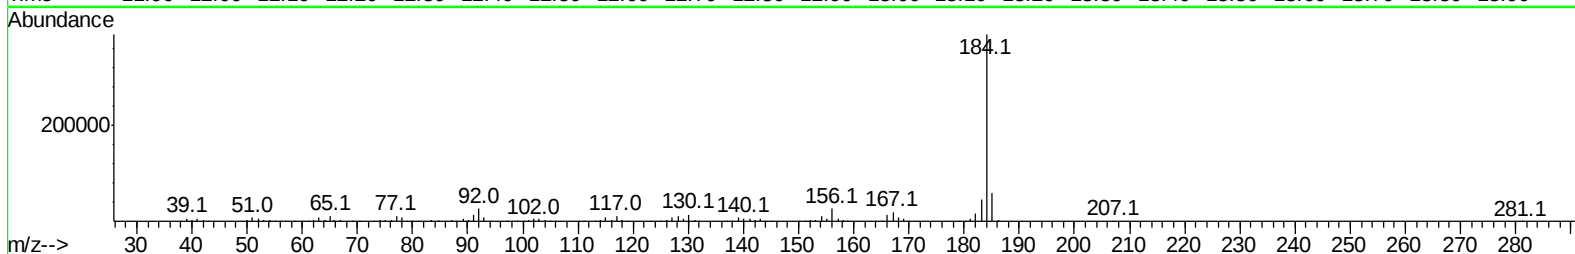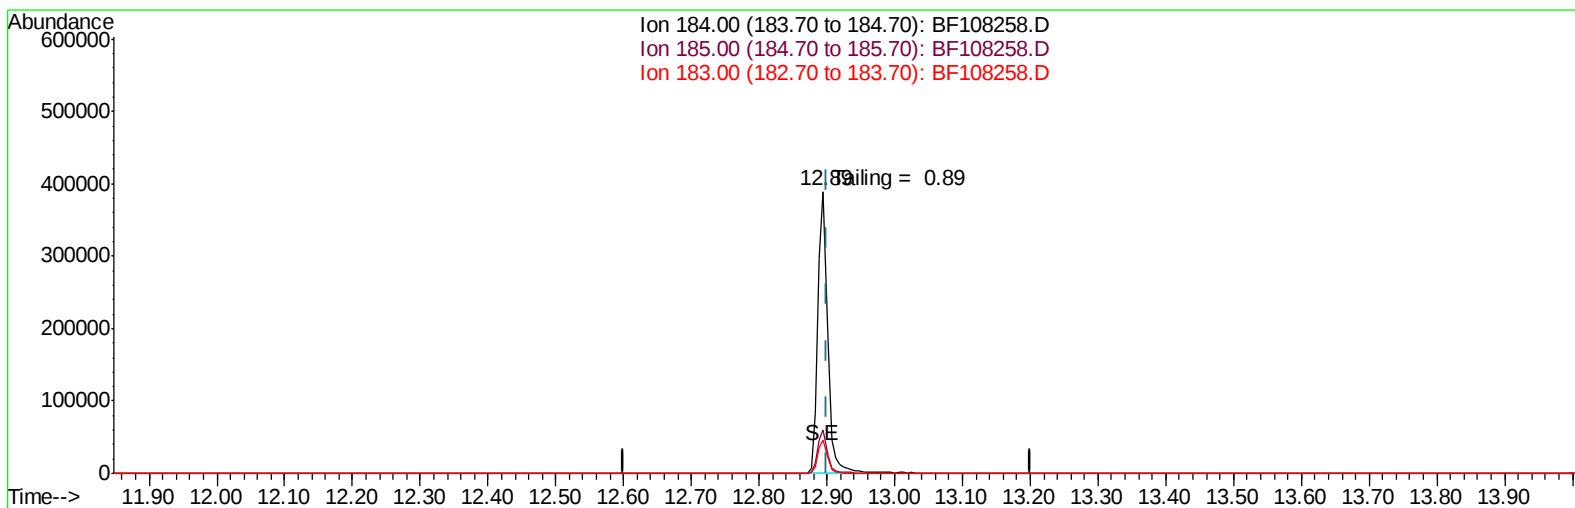

TIC: BF108258.D

(76) Benzidine

12.895min (-0.006) 0.00ng

response 382443

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.34
183.00	11.60	11.99
0.00	0.00	0.00