


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081718\
 Data File : BF108231.D
 Acq On : 17 Aug 2018 9:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

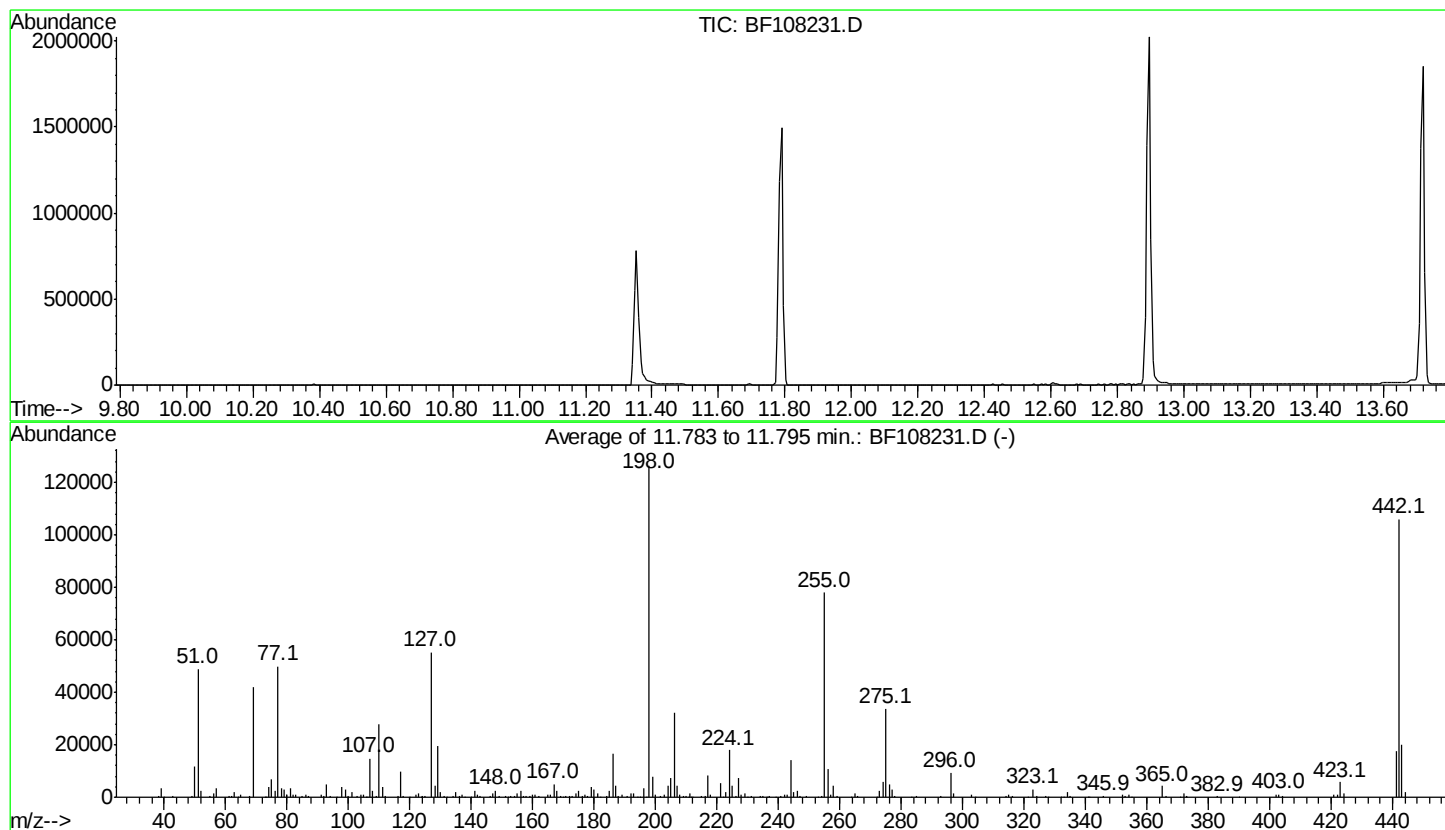

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	48949	PASS
68	69	0.00	2	1.6	670	PASS
69	198	0.00	100	33.4	42143	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.7	55242	PASS
197	198	0.00	2	0.1	101	PASS
198	198	100	100	100.0	126362	PASS
199	198	5	9	6.2	7867	PASS
275	198	10	60	26.7	33741	PASS
365	198	1	100	3.5	4383	PASS
441	198	0.01	100	13.8	17379	PASS
442	198	50	100	83.9	106058	PASS
443	442	15	24	19.1	20231	PASS