

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081719\
 Data File : BF116356.D
 Acq On : 17 Aug 2019 14:44
 Operator : HP/JU
 Sample : K4391-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 N-WALL-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.439	567	570	603	rBV	2188536	2533568	84.63%	9.715%
2	6.451	738	742	761	rBV	2544463	2745083	91.69%	10.526%
3	6.581	761	764	779	rVB	2793997	2668909	89.15%	10.234%
4	6.810	800	803	815	rBV	840417	771078	25.76%	2.957%
5	6.963	826	829	847	rBV	2193716	2073140	69.25%	7.949%
6	7.375	895	899	925	rBV	1670808	1712787	57.21%	6.567%
7	8.092	1017	1021	1037	rBV	917224	996257	33.28%	3.820%
8	9.163	1199	1203	1215	rBV	3097370	2993737	100.00%	11.479%
9	9.557	1267	1270	1284	rBV	244718	232021	7.75%	0.890%
10	9.839	1315	1318	1332	rVB	1371967	1164607	38.90%	4.466%
11	10.633	1449	1453	1469	rBV	1702194	1823364	60.91%	6.991%
12	11.327	1568	1571	1580	rBV	1288377	1156622	38.63%	4.435%
13	11.392	1580	1582	1588	rVB2	49837	46860	1.57%	0.180%
14	11.851	1656	1660	1663	rBV	46830	53855	1.80%	0.206%
15	12.904	1835	1839	1843	rBV	3065069	2758161	92.13%	10.576%
16	13.127	1872	1877	1882	rBV	31651	34097	1.14%	0.131%
17	13.792	1986	1990	2009	rBV2	130884	291215	9.73%	1.117%
18	13.968	2017	2020	2032	rBV	906066	903228	30.17%	3.463%
19	14.415	2092	2096	2099	rBV	38966	37300	1.25%	0.143%
20	14.709	2142	2146	2150	rBV	48029	51569	1.72%	0.198%
21	14.786	2155	2159	2163	rBV	38250	37745	1.26%	0.145%
22	15.039	2197	2202	2209	rBV	53060	60305	2.01%	0.231%
23	15.427	2259	2268	2283	rBV	520684	816666	27.28%	3.131%
24	15.821	2330	2335	2339	rBV	44160	63194	2.11%	0.242%
25	16.303	2412	2417	2427	rVB3	27837	54652	1.83%	0.210%


Sum of corrected areas: 26080020

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081719\
Data File : BF116356.D
Acq On : 17 Aug 2019 14:44
Operator : HP/JU
Sample : K4391-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
N-WALL-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

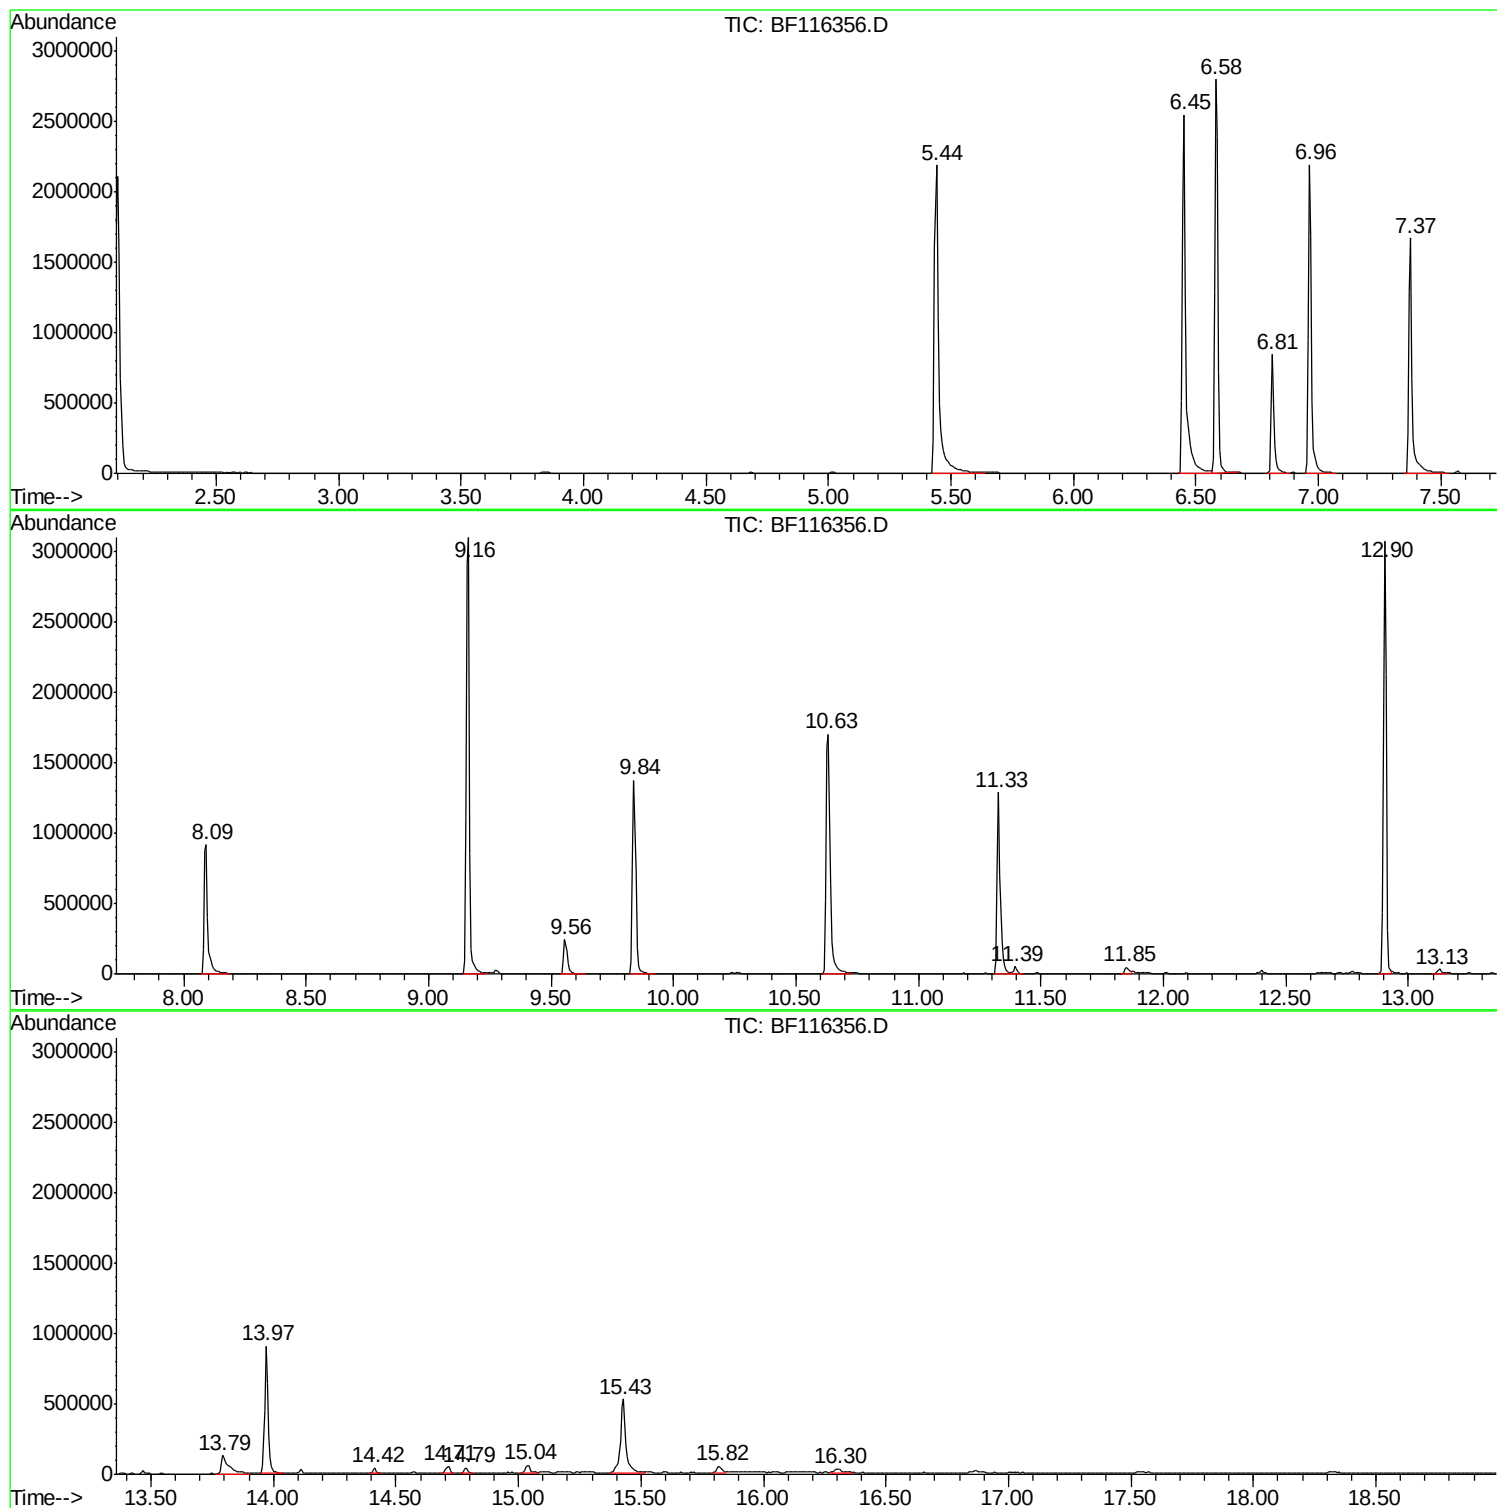

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081719\
Data File : BF116356.D
Acq On : 17 Aug 2019 14:44
Operator : HP/JU
Sample : K4391-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
N-WALL-1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.58	69.23 ng	2668910	1,4-Dichlorobenzene-d4	6.81

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	10
2		Xenon	132	Xe	007440-63-3	9
3		Bicvclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9

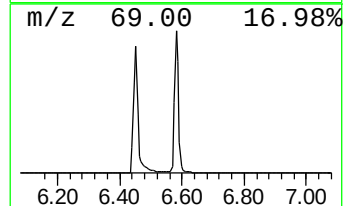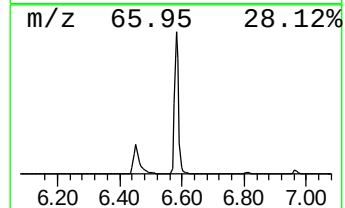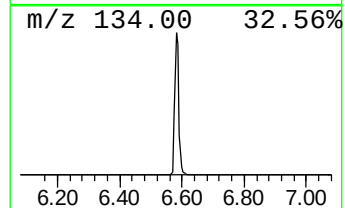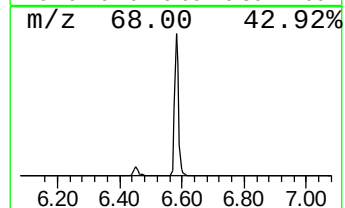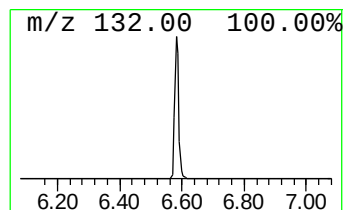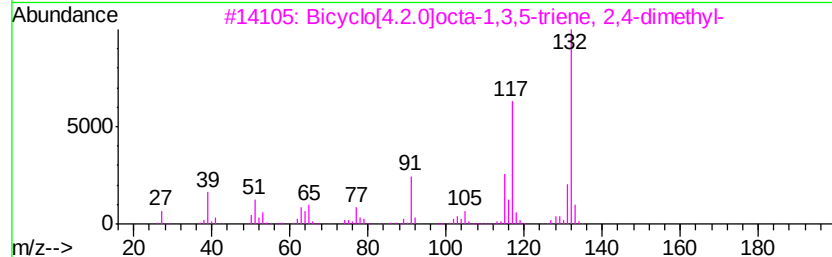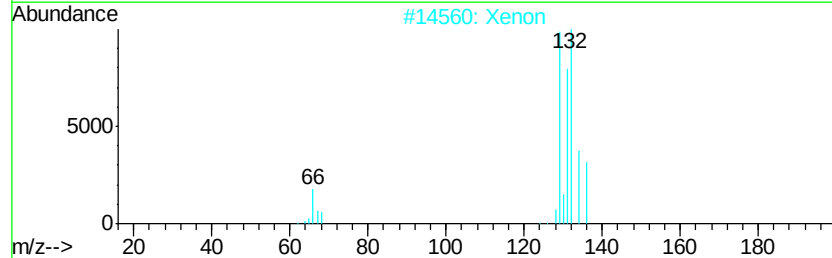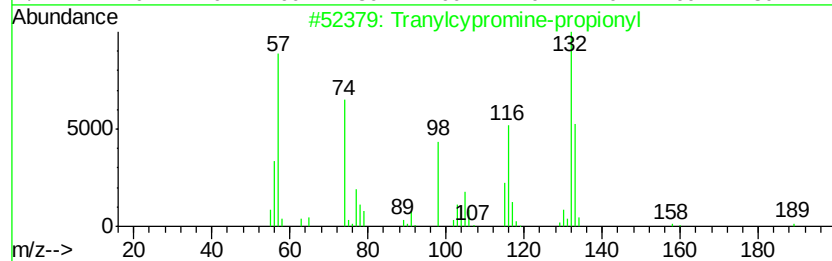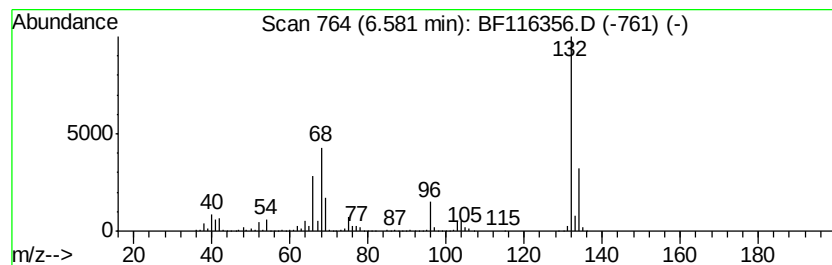

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081719\
Data File : BF116356.D
Acq On : 17 Aug 2019 14:44
Operator : HP/JU
Sample : K4391-01
Misc :
ALS Vial : 10 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
N-WALL-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Ethanol, 2-(tetradecyloxy)- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.		
13.79	6.45 ng	291215	Chrysene-d12	13.97		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	91
2		Pentafluoropropionic acid, octadecyl ester	416	C21H37F5O2	959261-25-7	87
3		Pentafluoropropionic acid, heptadecyl ester	402	C20H35F5O2	959218-78-1	81
4		Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	81
5		Carbonic acid, octadecyl 2,2,2-trifluoroethyl ester	444	C21H39Cl3O3	1000314-56-3	81

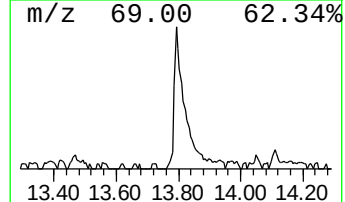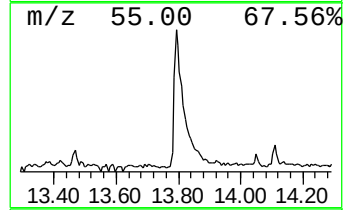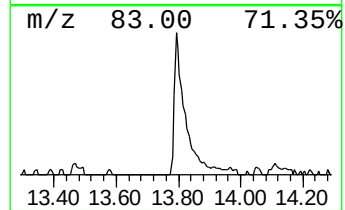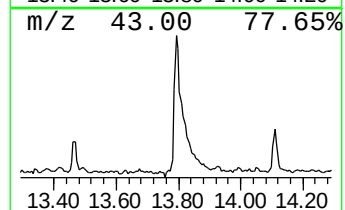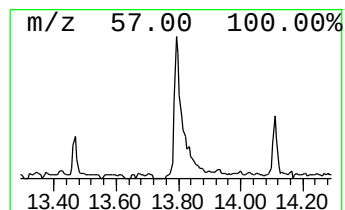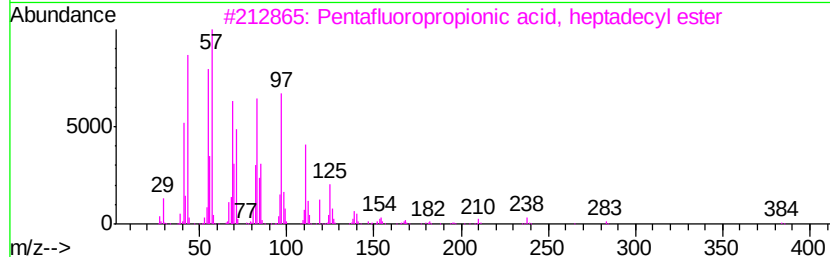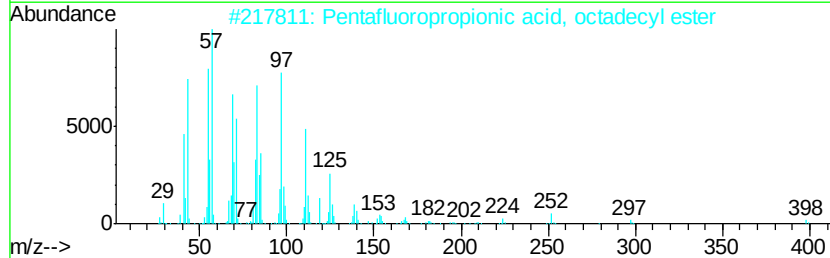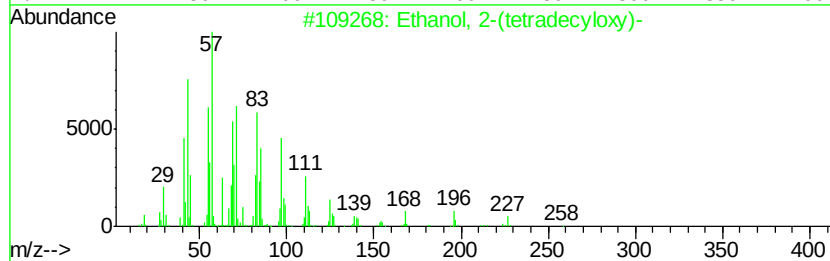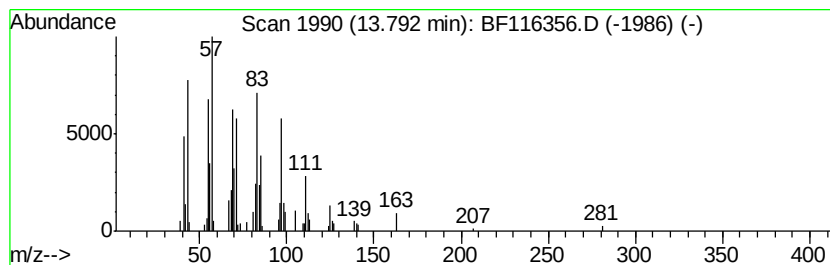

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081719\
Data File : BF116356.D
Acq On : 17 Aug 2019 14:44
Operator : HP/JU
Sample : K4391-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
N-WALL-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.58	6.58	69.2	ng	2668910	1	6.81	771078	20.0
Ethanol, 2-(tetra...	13.79	6.5	ng	291215	5	13.97	903228	20.0