


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081719\
 Data File : BF116347.D
 Acq On : 17 Aug 2019 10:37
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

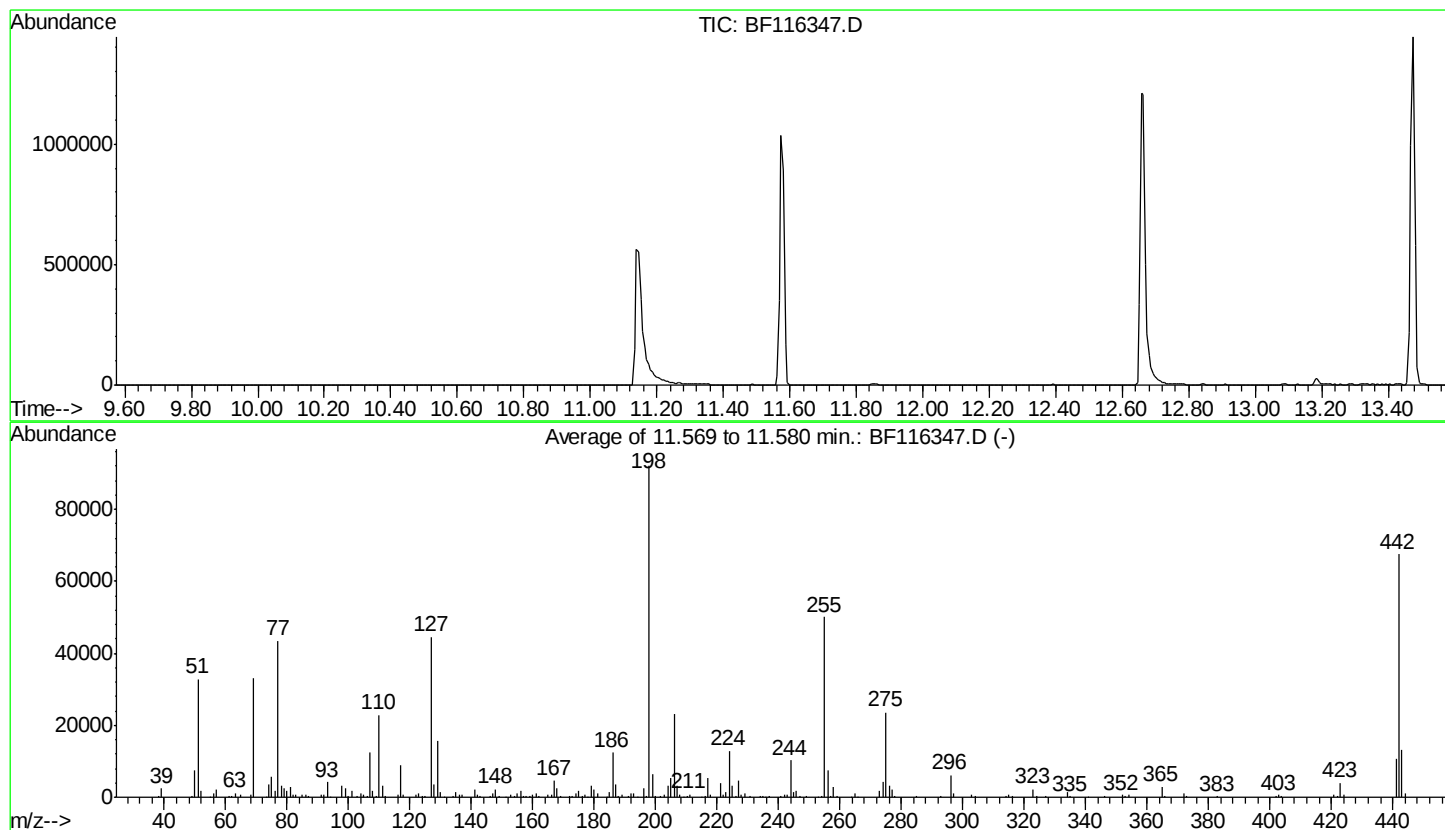

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	32773	PASS
68	69	0.00	2	1.8	579	PASS
69	198	0.00	100	35.8	32946	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	44509	PASS
197	198	0.00	2	0.5	452	PASS
198	198	100	100	100.0	92120	PASS
199	198	5	9	6.8	6238	PASS
275	198	10	60	25.6	23579	PASS
365	198	1	100	3.2	2924	PASS
441	198	0.01	100	11.5	10583	PASS
442	198	50	100	73.3	67516	PASS
443	442	15	24	19.3	13049	PASS