


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081719\
 Data File : BF116371.D
 Acq On : 18 Aug 2019 00:40
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

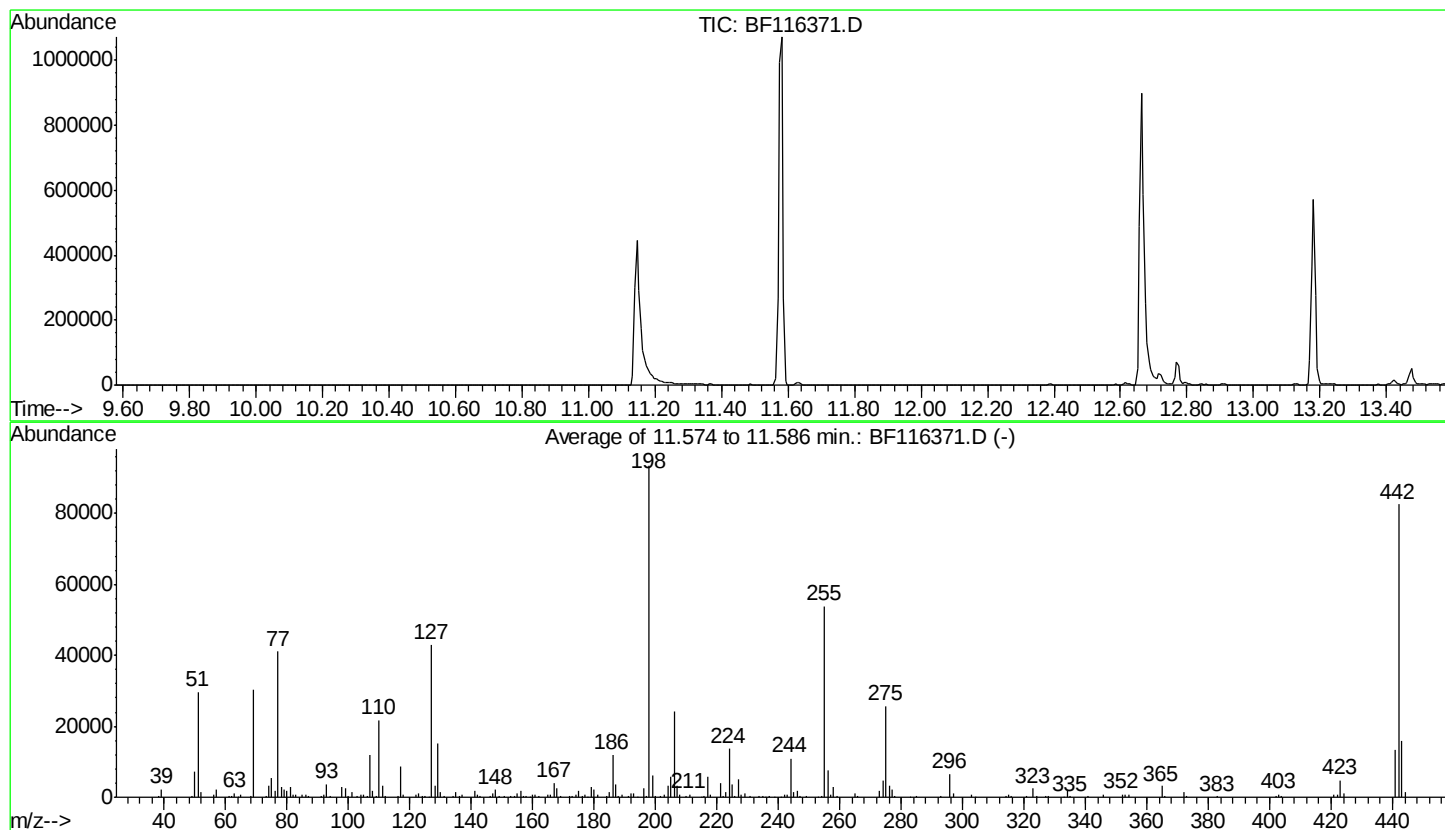

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	29726	PASS
68	69	0.00	2	1.5	450	PASS
69	198	0.00	100	32.5	30412	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	43056	PASS
197	198	0.00	2	0.5	423	PASS
198	198	100	100	100.0	93464	PASS
199	198	5	9	6.6	6204	PASS
275	198	10	60	27.5	25699	PASS
365	198	1	100	3.4	3199	PASS
441	198	0.01	100	14.4	13491	PASS
442	198	50	100	88.4	82597	PASS
443	442	15	24	19.1	15812	PASS