
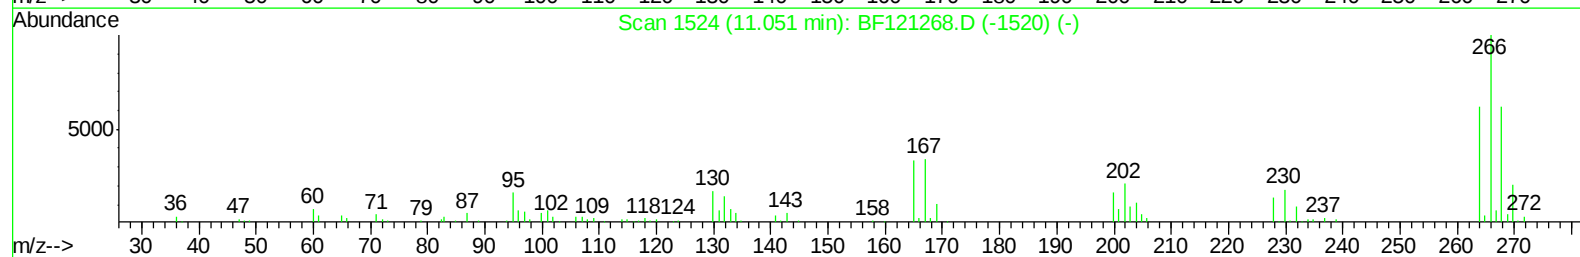
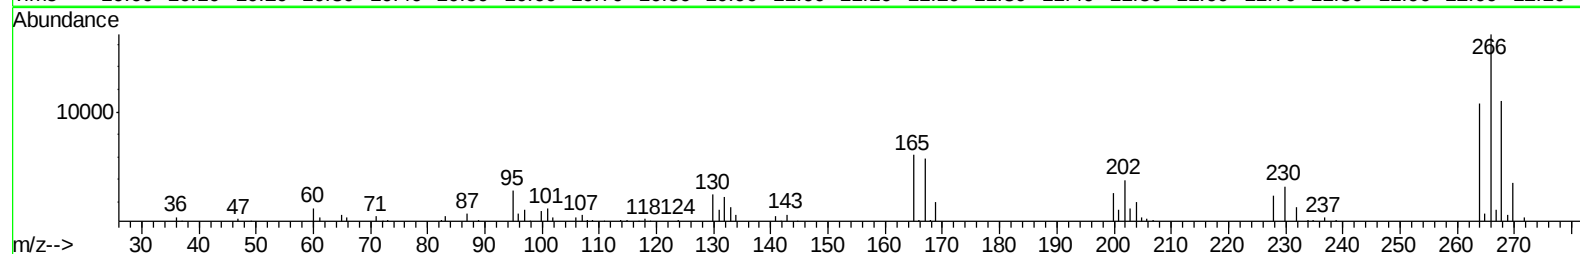


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081720\
Data File : BF121299.D
Acq On : 17 Aug 2020 8:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 07:19:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 10:52:06 2020
Response via : Initial Calibration

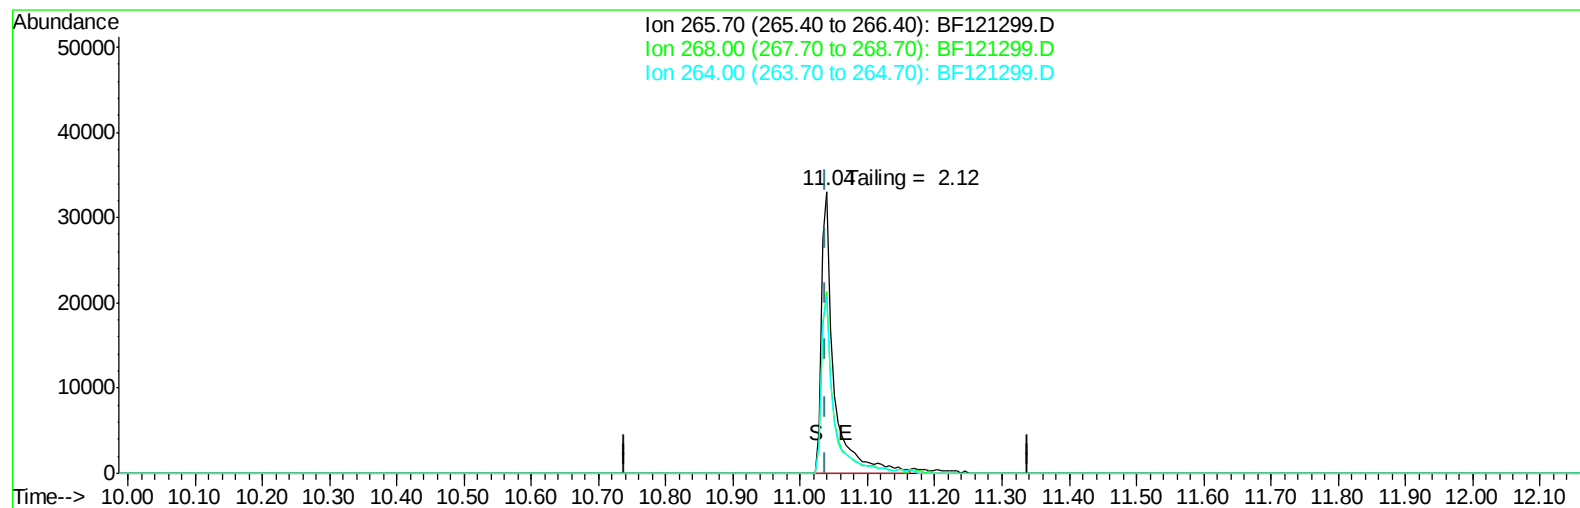

TIC: BF121299.D

(70) Pentachlorophenol (C)




11.039min (-0.000) 9053.88ng

response 43694

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.68
264.00	61.70	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081720\
Data File : BF121299.D
Acq On : 17 Aug 2020 8:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 07:19:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 10:52:06 2020
Response via : Initial Calibration

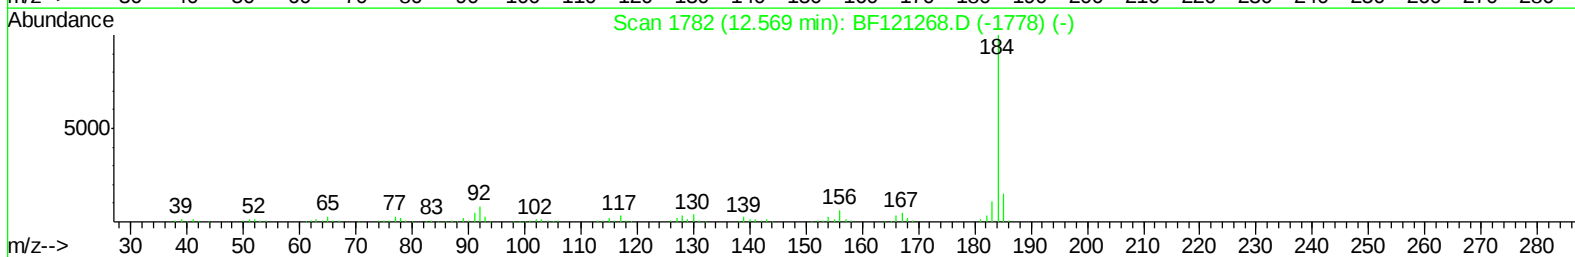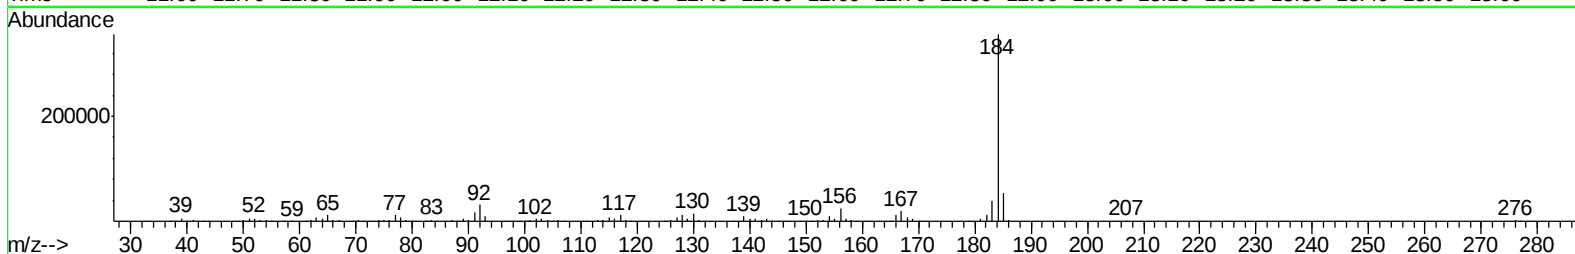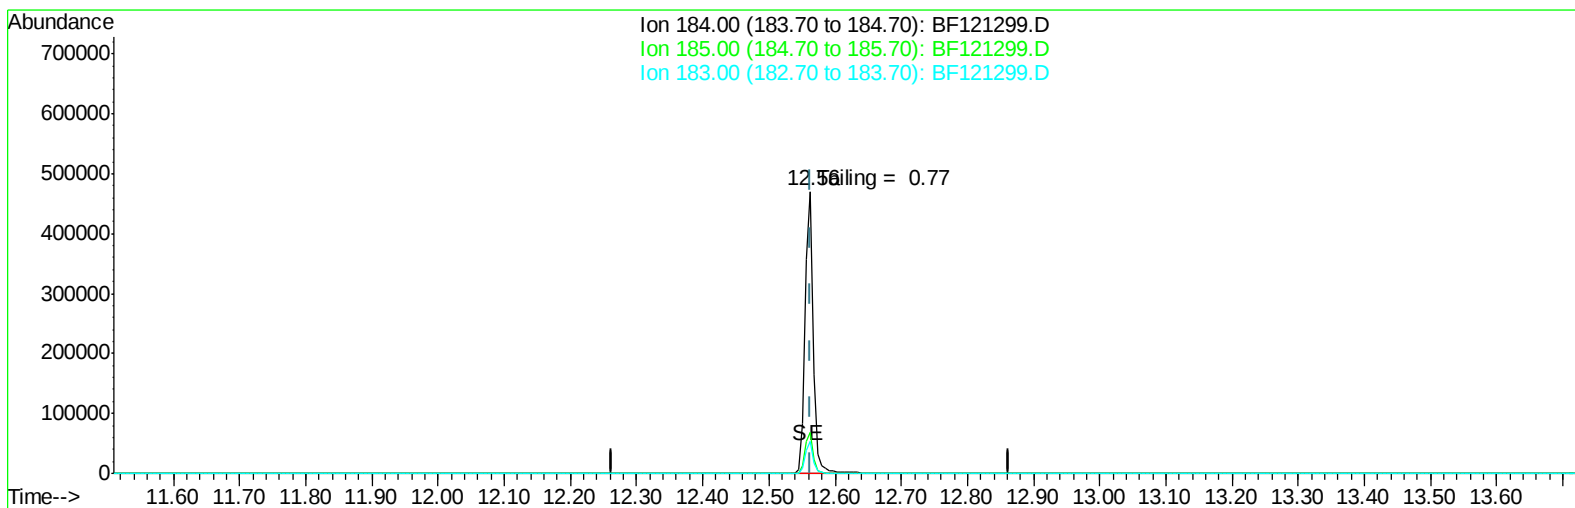

TIC: BF121299.D

(77) Benzidine

12.563min (-0.000) 17905.77ng

response 411410

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.61
183.00	10.80	11.19
0.00	0.00	0.00