

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081720\
 Data File : BF121314.D
 Acq On : 17 Aug 2020 17:20
 Operator : JU/CG
 Sample : L3508-19 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-08-081420

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.869	470	473	481	rBB2	25668	28450	3.33%	0.358%
2	5.304	544	547	557	rBV	173930	187506	21.96%	2.361%
3	5.945	654	656	662	rBB	9484	10042	1.18%	0.126%
4	6.234	702	705	708	rBV2	8879	9464	1.11%	0.119%
5	6.339	720	723	737	rBV	235007	264308	30.95%	3.328%
6	6.545	753	758	763	rBV2	28128	28792	3.37%	0.363%
7	6.704	781	785	793	rBV	657511	524226	61.39%	6.601%
8	7.263	877	880	885	rBV	199043	182744	21.40%	2.301%
9	7.310	885	888	891	rVB	30647	26848	3.14%	0.338%
10	7.986	999	1003	1010	rBV	820186	707644	82.87%	8.911%
11	8.416	1071	1076	1081	rBV	9864	10243	1.20%	0.129%
12	8.586	1102	1105	1109	rBV	21213	18465	2.16%	0.233%
13	9.063	1183	1186	1197	rBV	517774	410193	48.04%	5.165%
14	9.151	1197	1201	1205	rVB	25373	23380	2.74%	0.294%
15	9.398	1240	1243	1246	rBV2	10058	10220	1.20%	0.129%
16	9.463	1250	1254	1257	rBV	75009	76013	8.90%	0.957%
17	9.604	1274	1278	1283	rVB	13055	12062	1.41%	0.152%
18	9.674	1283	1290	1295	rBV2	29608	43419	5.08%	0.547%
19	9.739	1297	1301	1311	rVB	928984	795225	93.13%	10.013%
20	10.174	1372	1375	1378	rVB	26853	21930	2.57%	0.276%
21	10.398	1407	1413	1415	rBV	18556	18414	2.16%	0.232%
22	10.527	1430	1435	1439	rBV	117899	111205	13.02%	1.400%
23	10.651	1453	1456	1460	rBV2	35819	48300	5.66%	0.608%
24	11.098	1529	1532	1534	rBV2	32590	26723	3.13%	0.336%
25	11.127	1534	1537	1543	rVB2	21411	25094	2.94%	0.316%
26	11.221	1549	1553	1560	rBV	956007	832534	97.50%	10.483%
27	11.298	1564	1566	1570	rVB	16481	15952	1.87%	0.201%
28	11.521	1601	1604	1607	rBV	38341	28521	3.34%	0.359%
29	11.551	1607	1609	1615	rVB2	8452	11269	1.32%	0.142%
30	11.727	1636	1639	1641	rBV2	11031	10596	1.24%	0.133%
31	11.751	1641	1643	1647	rVB	12474	10201	1.19%	0.128%
32	11.798	1647	1651	1653	rBV4	7494	10241	1.20%	0.129%
33	11.833	1654	1657	1660	rVV4	13240	11704	1.37%	0.147%
34	11.927	1670	1673	1676	rBV	37960	32981	3.86%	0.415%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081720\
 Data File : BF121314.D
 Acq On : 17 Aug 2020 17:20
 Operator : JU/CG
 Sample : L3508-19 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-08-081420

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.086	1697	1700	1703	rBV5	9001	14065	1.65%	0.177%
36	12.151	1708	1711	1713	rVV	13192	15719	1.84%	0.198%
37	12.204	1716	1720	1724	rVV7	12236	21759	2.55%	0.274%
38	12.268	1729	1731	1734	rBV	22300	22605	2.65%	0.285%
39	12.315	1734	1739	1744	rBV2	44771	51294	6.01%	0.646%
40	12.357	1744	1746	1750	rVB4	11191	13540	1.59%	0.170%
41	12.392	1750	1752	1755	rBV3	11456	14388	1.68%	0.181%
42	12.433	1755	1759	1762	rBV	109145	101710	11.91%	1.281%
43	12.527	1772	1775	1777	rBV2	23034	20832	2.44%	0.262%
44	12.586	1783	1785	1788	rBV3	15582	18420	2.16%	0.232%
45	12.657	1792	1797	1800	rVV	115587	118695	13.90%	1.495%
46	12.686	1800	1802	1805	rVV	47287	40659	4.76%	0.512%
47	12.721	1805	1808	1811	rVV3	12634	15160	1.78%	0.191%
48	12.768	1814	1816	1818	rBV2	10178	11495	1.35%	0.145%
49	12.804	1818	1822	1827	rVB	520914	441872	51.75%	5.564%
50	12.986	1851	1853	1857	rVB2	33354	31110	3.64%	0.392%
51	13.045	1857	1863	1867	rBV2	53024	77205	9.04%	0.972%
52	13.092	1868	1871	1873	rBV3	22385	22497	2.63%	0.283%
53	13.386	1918	1921	1923	rBV	40475	37135	4.35%	0.468%
54	13.498	1938	1940	1944	rVB2	21051	24132	2.83%	0.304%
55	13.709	1974	1976	1984	rVB2	60190	82005	9.60%	1.033%
56	13.857	1996	2001	2004	rBV	784204	853888	100.00%	10.752%
57	13.880	2004	2005	2008	rVB	86588	52239	6.12%	0.658%
58	14.027	2028	2030	2035	rVB2	42684	40746	4.77%	0.513%
59	14.333	2080	2082	2085	rVB2	37482	30229	3.54%	0.381%
60	14.868	2169	2173	2181	rVB	129417	216906	25.40%	2.731%
61	15.151	2219	2221	2226	rVB	73105	75444	8.84%	0.950%
62	15.209	2228	2231	2236	rVB	109668	131574	15.41%	1.657%
63	15.268	2237	2241	2245	rBV	651762	759331	88.93%	9.561%


Sum of corrected areas: 7941563

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081720\
Data File : BF121314.D
Acq On : 17 Aug 2020 17:20
Operator : JU/CG
Sample : L3508-19 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TR-08-081420

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

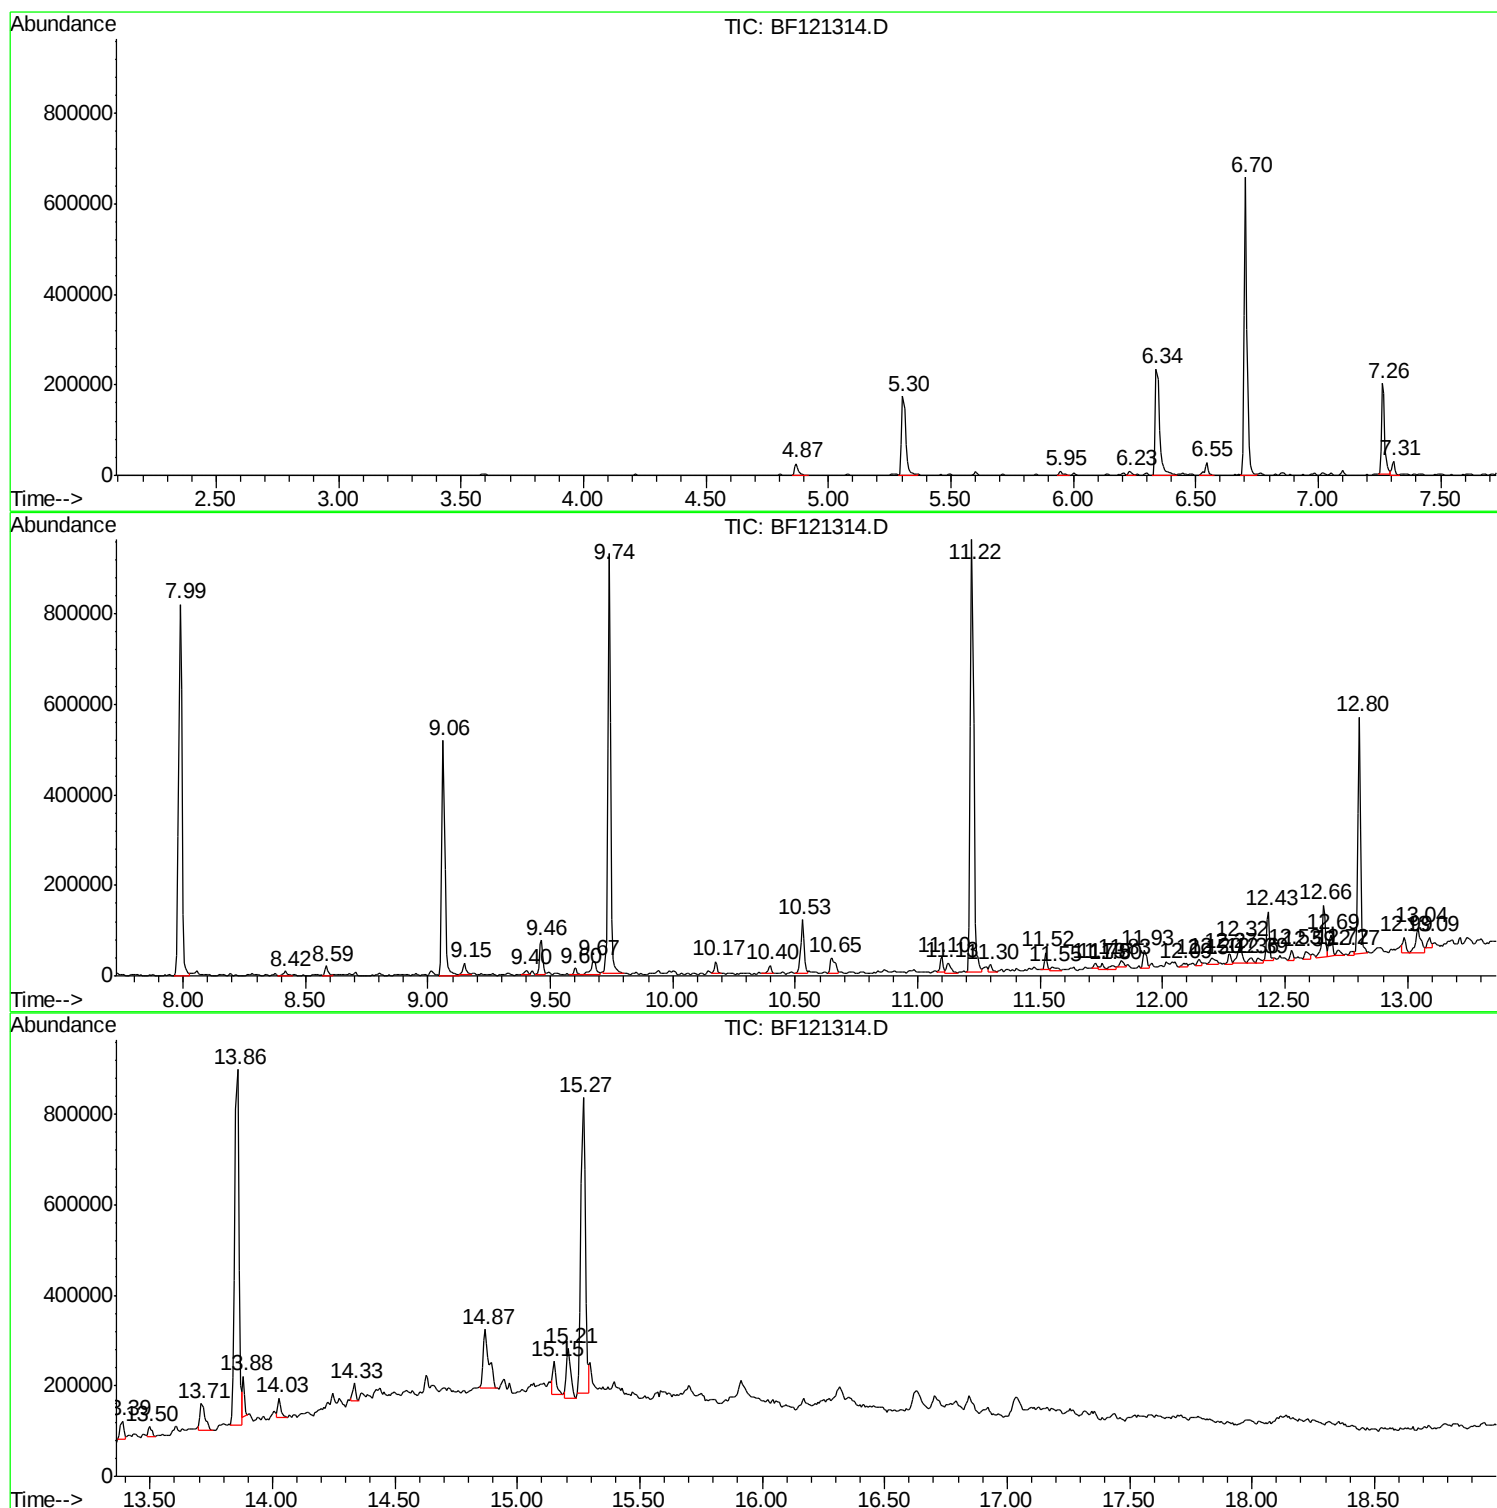

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081720\
Data_File : BF121314.D
Acq_On : 17 Aug 2020 17:200
Operator : JU/CGG
Sample : L3508-19-2XX
Misc :
ALS_Vial : 16 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
TR-08-081420

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
