


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081720\
 Data File : BF121299.D
 Acq On : 17 Aug 2020 8:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 10:52:06 2020

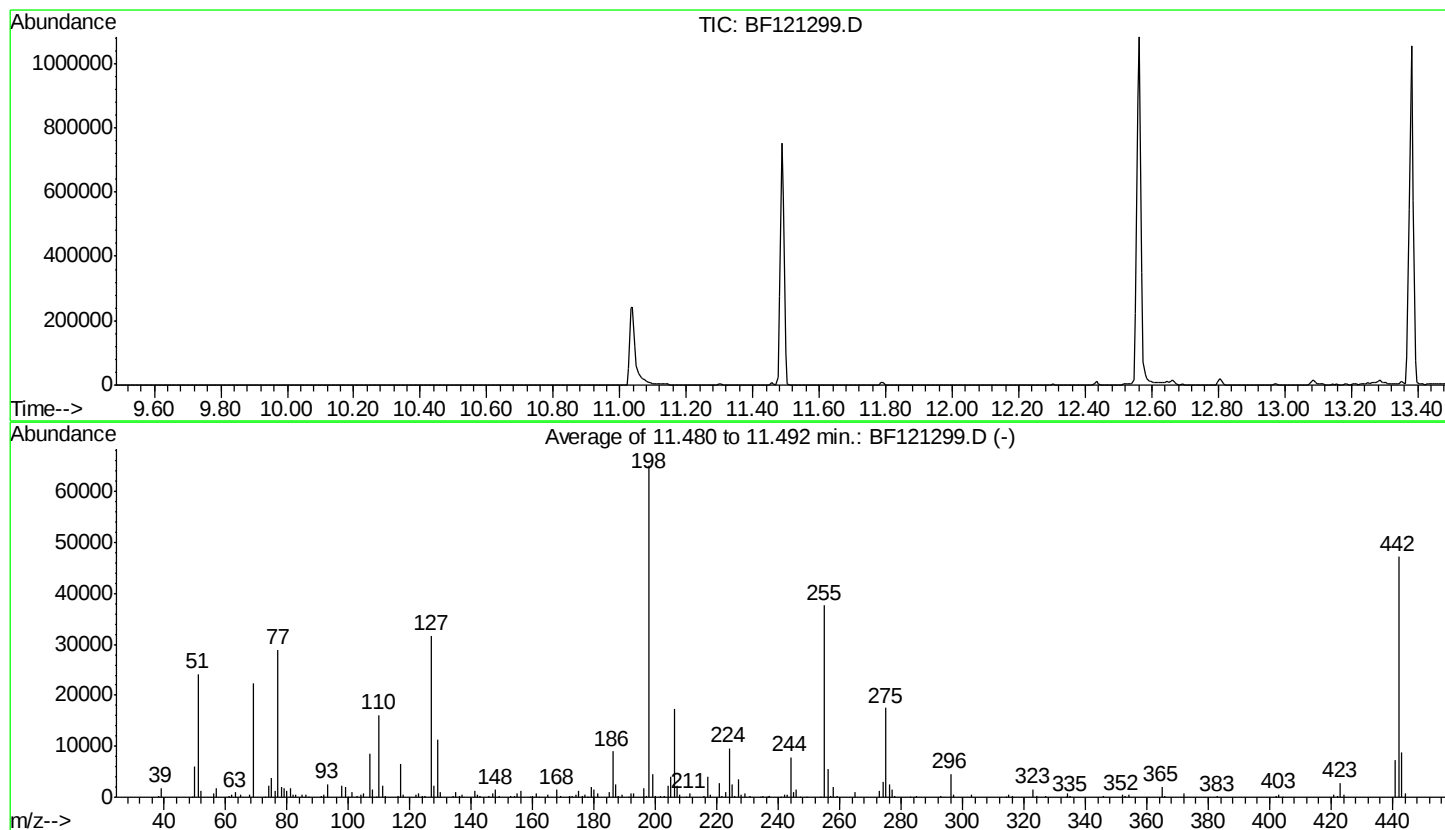

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	24181	PASS
68	69	0.00	2	1.8	407	PASS
69	198	0.00	100	34.2	22294	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	31720	PASS
197	198	0.00	2	0.6	364	PASS
198	198	100	100	100.0	65101	PASS
199	198	5	9	6.9	4478	PASS
275	198	10	60	27.0	17590	PASS
365	198	1	100	3.2	2087	PASS
441	198	0.01	100	11.4	7395	PASS
442	198	50	100	72.6	47239	PASS
443	442	15	24	18.7	8851	PASS