
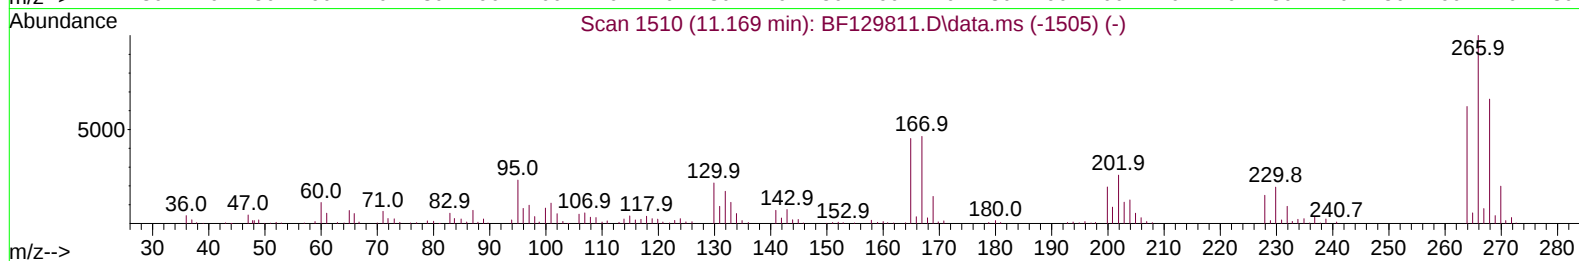
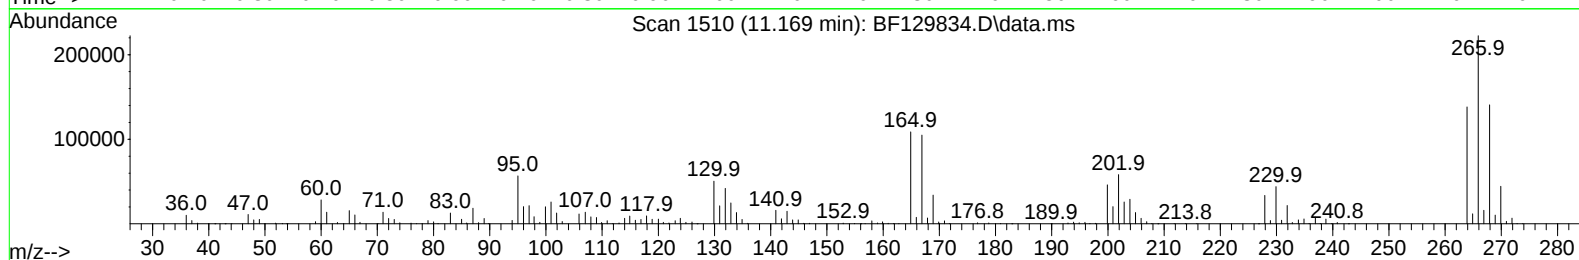


Quant Time: Aug 17 17:52:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

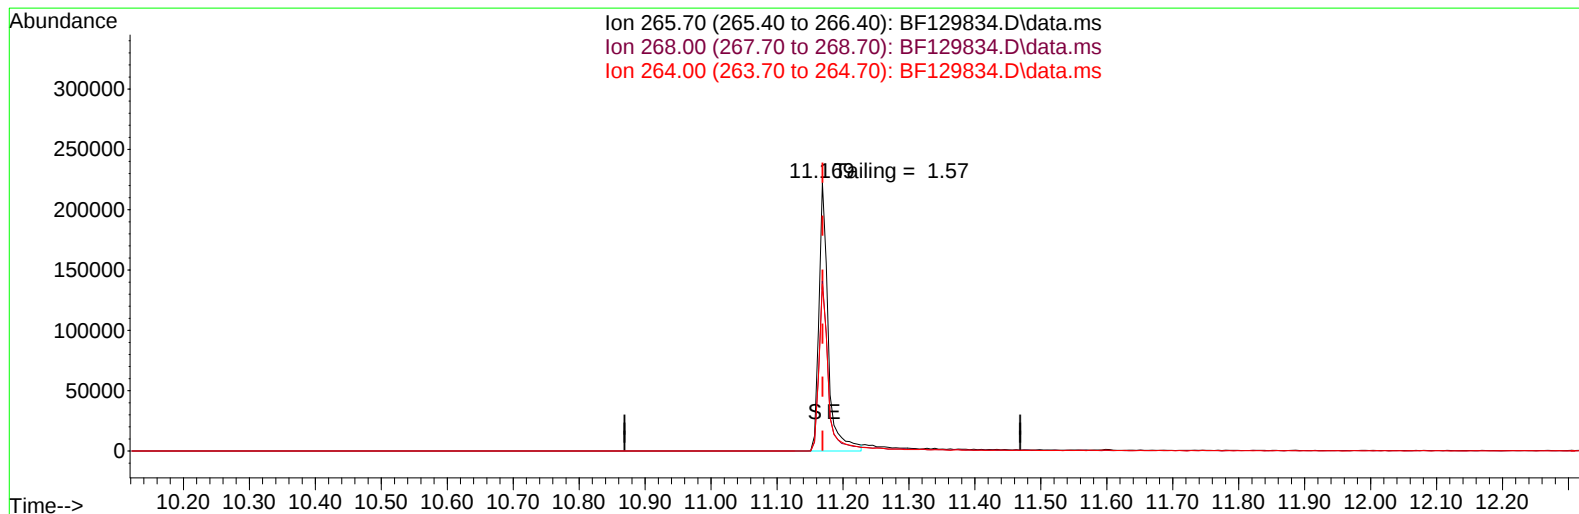

TIC: BF129834.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.000) 39446.68 ng

response 234488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.29
264.00	59.90	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129834.D
Acq On : 17 Aug 2022 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 17:52:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

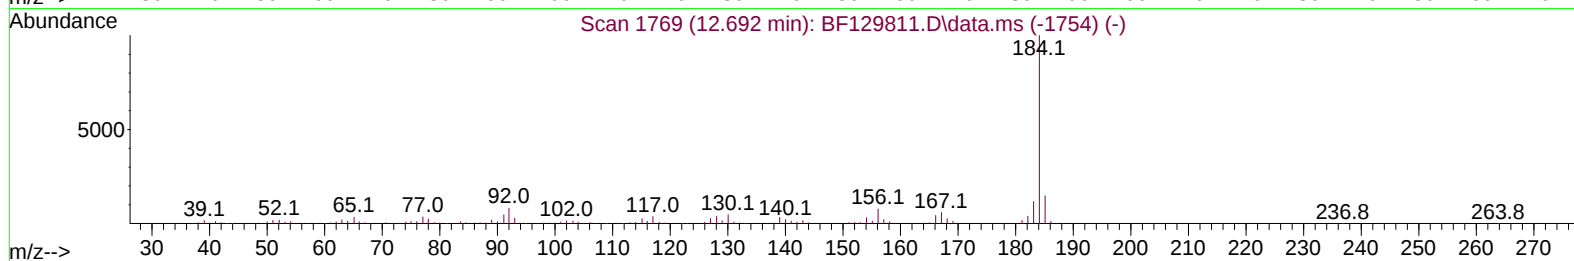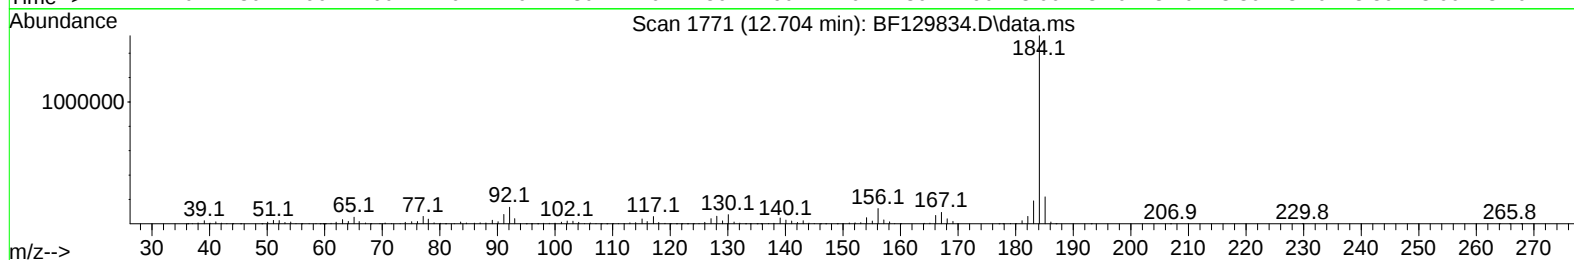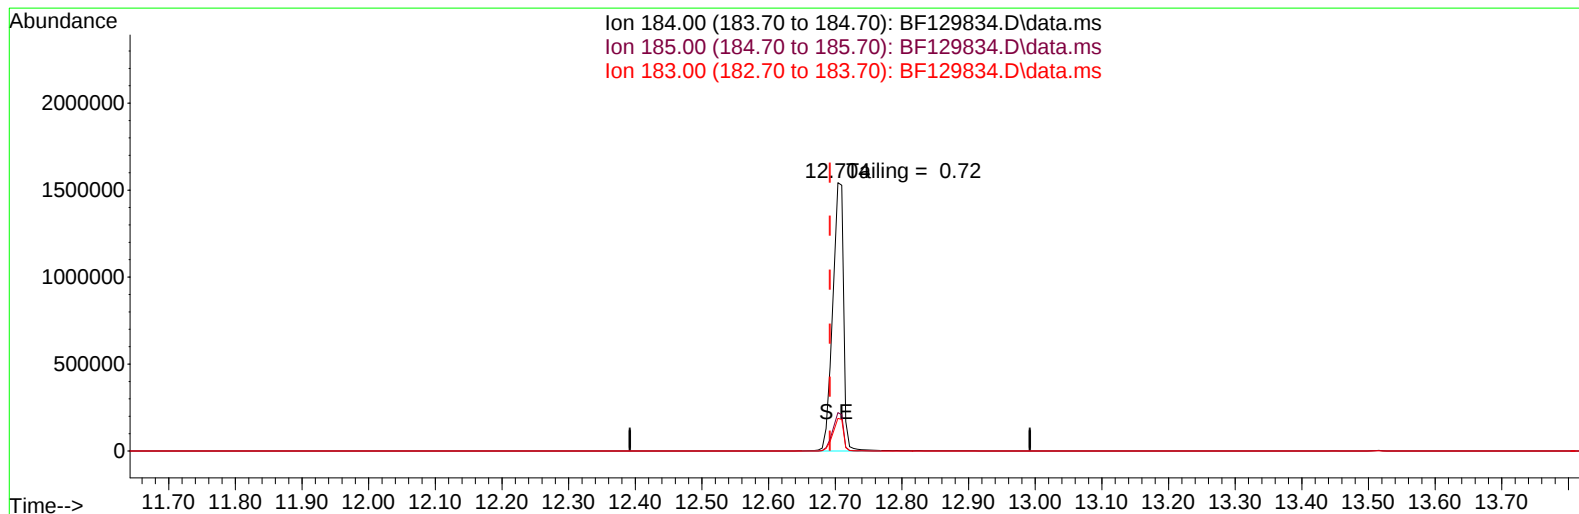

TIC: BF129834.D\data.ms

(77) Benzidine**12.704min (+ 0.012) 1070192.88 ng****response 1742463**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.34
183.00	11.80	12.15
0.00	0.00	0.00