

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
 Data File : BF129858.D
 Acq On : 17 Aug 2022 22:51
 Operator : CG\JU
 Sample : N4188-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	468	471	480	rBV	30742	44306	1.10%	0.169%
2	5.451	534	538	559	rBV	3582942	3655552	91.13%	13.921%
3	6.469	706	711	724	rBV	3713858	3710979	92.51%	14.132%
4	6.810	765	769	776	rBV	932434	772788	19.26%	2.943%
5	7.381	861	866	869	rBV	2363513	2407011	60.00%	9.166%
6	8.092	983	987	991	rBV	1178465	1051479	26.21%	4.004%
7	9.169	1164	1170	1173	rBV	4363134	4011559	100.00%	15.277%
8	9.798	1273	1277	1281	rBV	53849	48413	1.21%	0.184%
9	9.845	1281	1285	1289	rVV	1311067	1194634	29.78%	4.549%
10	10.645	1417	1421	1424	rBV	3080638	2653352	66.14%	10.105%
11	11.339	1535	1539	1542	rBV	1409017	1173382	29.25%	4.468%
12	11.457	1555	1559	1563	rVB	93128	78563	1.96%	0.299%
13	12.922	1804	1808	1811	rBV	4209156	3711287	92.51%	14.133%
14	13.804	1954	1958	1960	rBV	44462	44562	1.11%	0.170%
15	13.839	1960	1964	1974	rVB5	32750	86065	2.15%	0.328%
16	13.986	1985	1989	1992	rBV	1035137	915273	22.82%	3.486%
17	15.451	2231	2238	2245	rVB	559300	699891	17.45%	2.665%




Sum of corrected areas: 26259096

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129858.D
Acq On : 17 Aug 2022 22:51
Operator : CG\JU
Sample : N4188-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

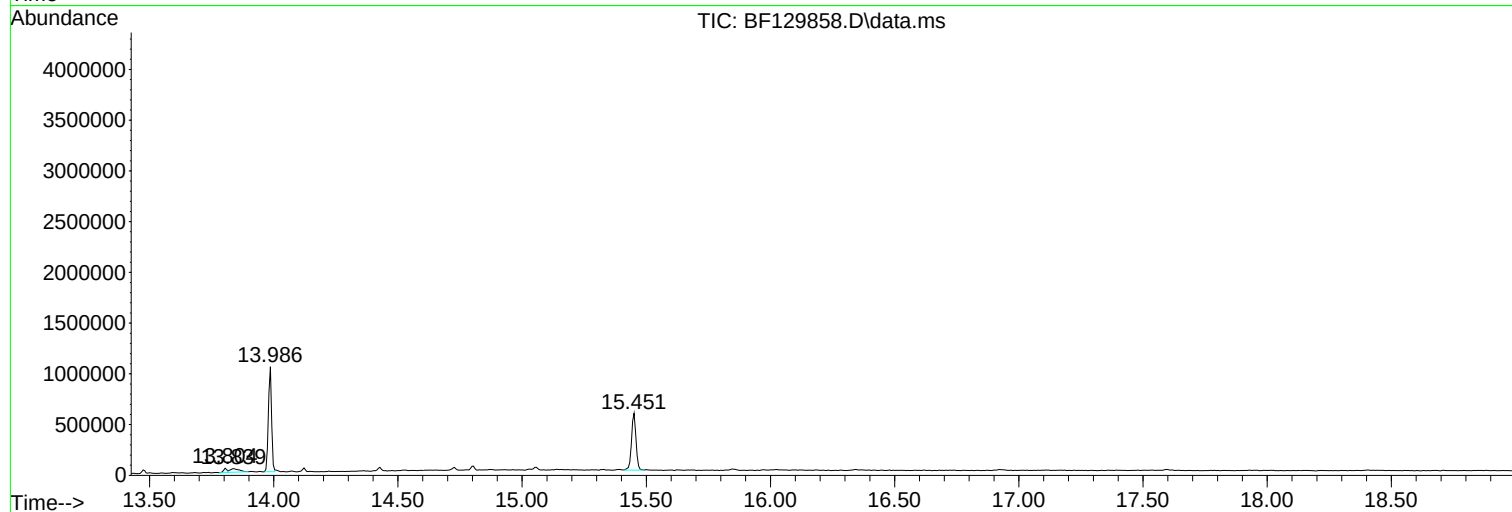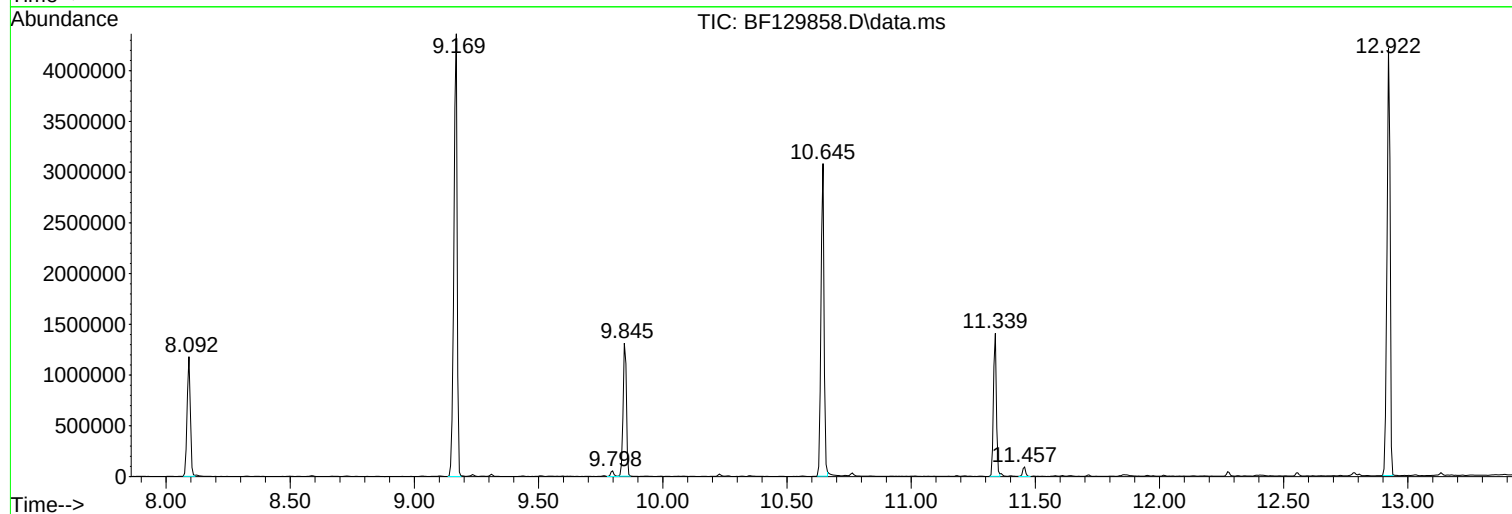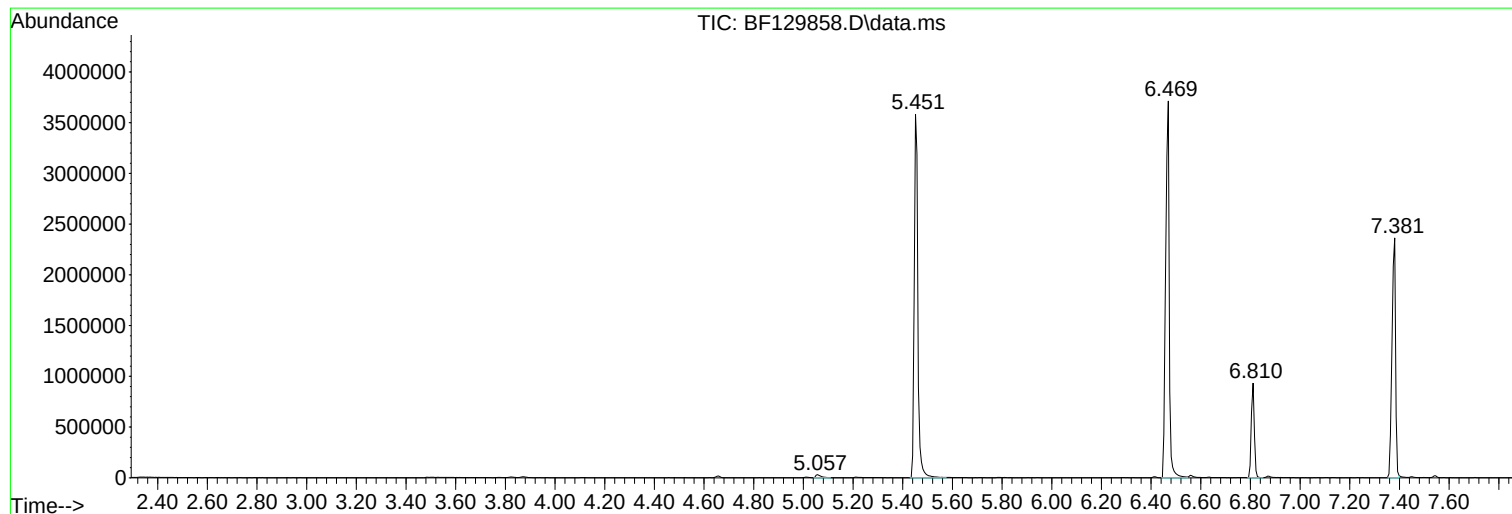

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129858.D
Acq On : 17 Aug 2022 22:51
Operator : CG\JU
Sample : N4188-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129858.D
Acq On : 17 Aug 2022 22:51
Operator : CG\JU
Sample : N4188-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------