


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
 Data File : BF129834.D
 Acq On : 17 Aug 2022 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 18 12:03:10 2022

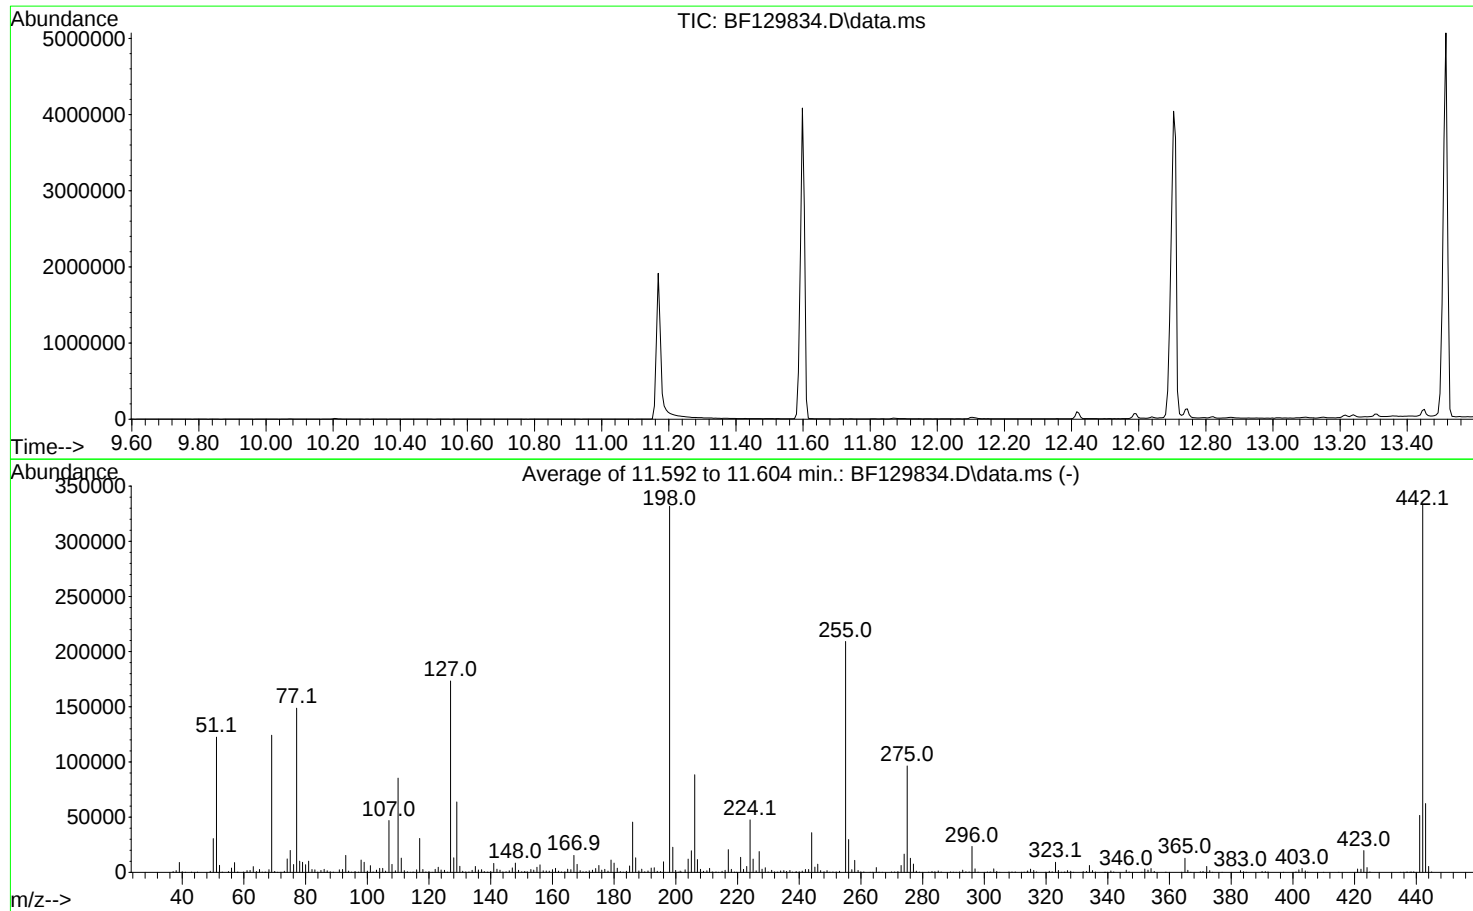




AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	122424	PASS
68	69	0.00	2	1.9	2348	PASS
69	198	0.00	100	37.4	124179	PASS
70	69	0.00	2	0.6	742	PASS
127	198	10	80	52.2	173320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	331733	PASS
199	198	5	9	6.9	22773	PASS
275	198	10	60	29.1	96435	PASS
365	198	1	100	3.8	12752	PASS
441	198	0.01	100	15.5	51499	PASS
442	442	50	100	100.0	333419	PASS
443	442	15	24	18.7	62293	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\  
Data File : BF129834.D  
Acq On    : 17 Aug 2022  09:11  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:52:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

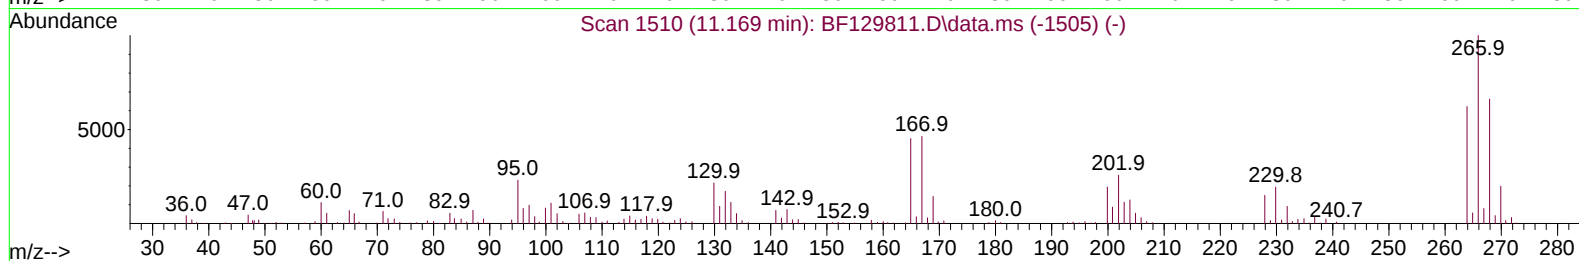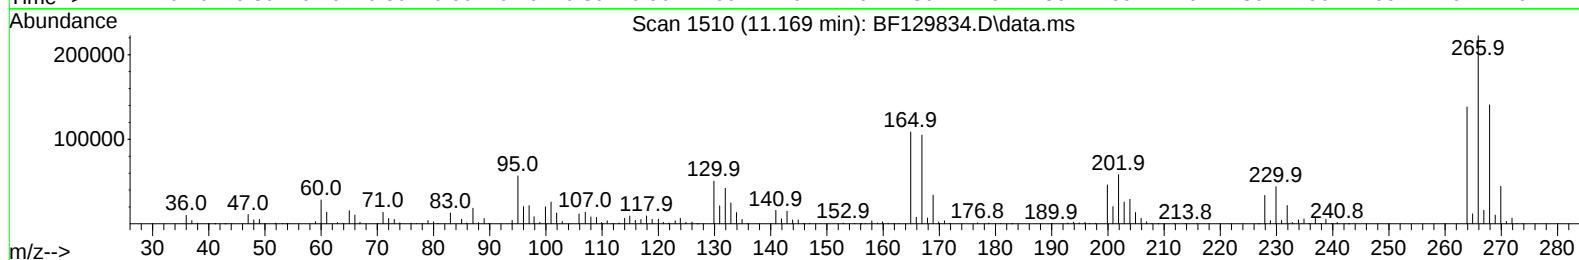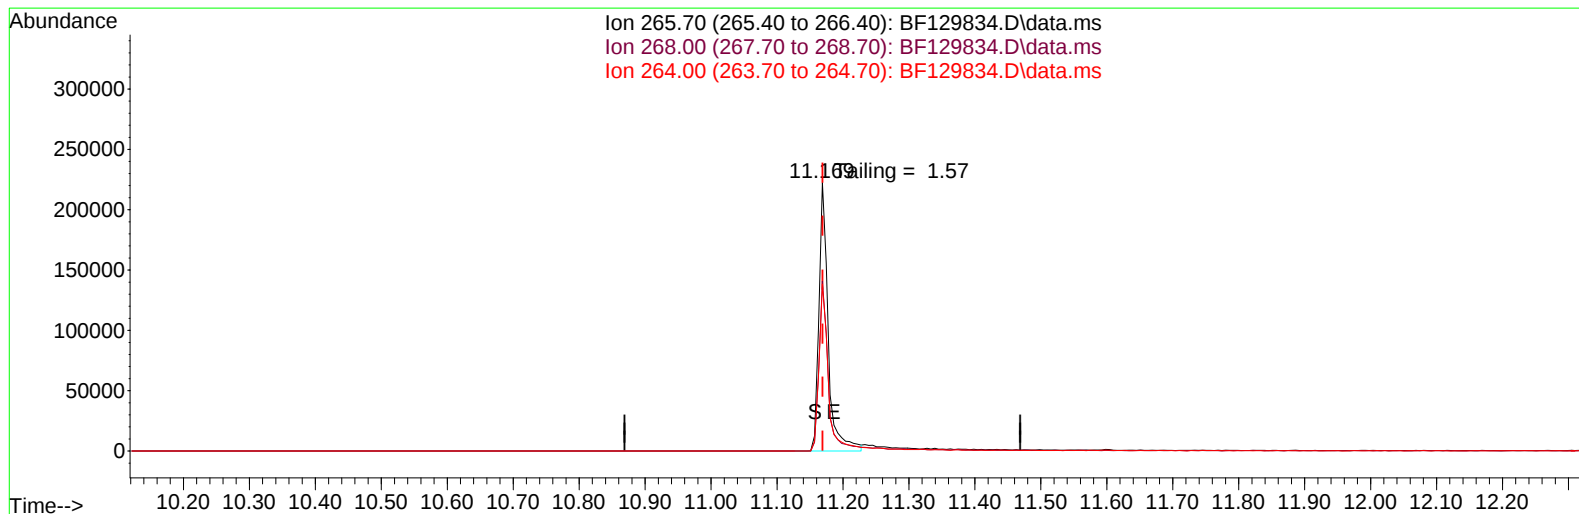

TIC: BF129834.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.000) 39446.68 ng




response 234488

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.29
264.00	59.90	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129834.D
Acq On : 17 Aug 2022 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:52:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

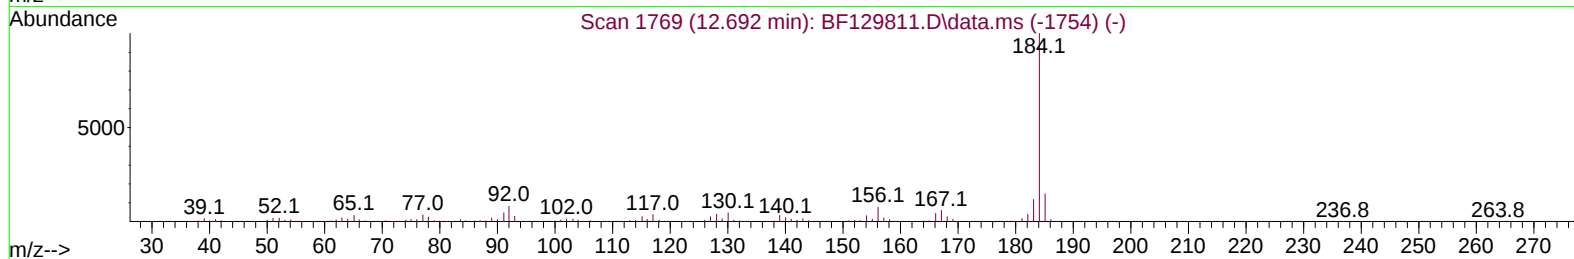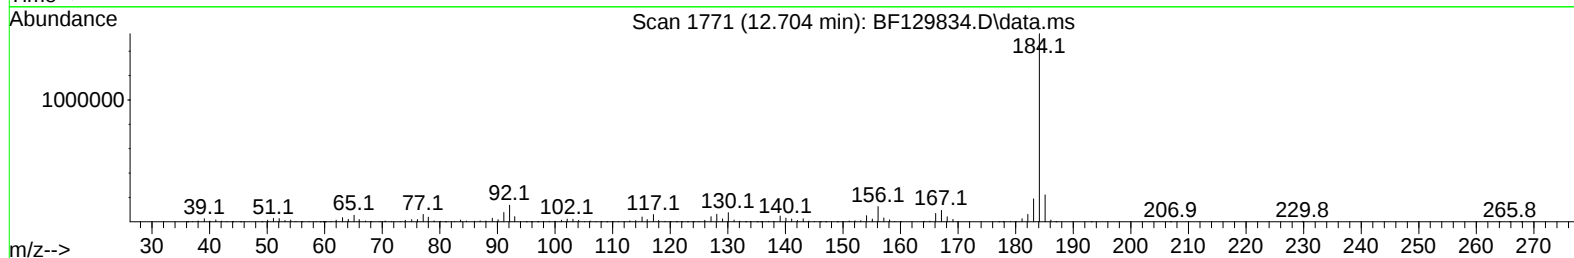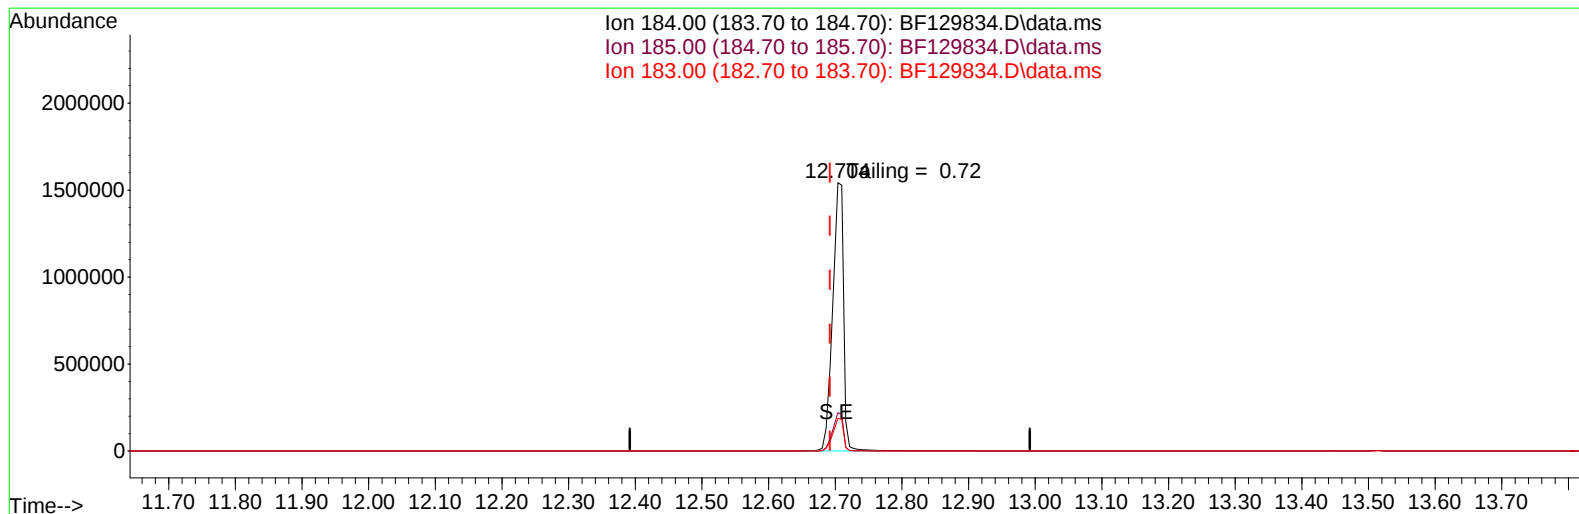

TIC: BF129834.D\data.ms

(77) Benzidine

12.704min (+ 0.012) 1070192.88 ng

response 1742463

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.34
183.00	11.80	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2022	BNA_F	<u>BF129834.D</u>
Compound Name	Response	Retention Time
DDT	856448	13.51
DDD	6439	13.21
DDE	2251	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8690	865138	1.00

Instrument :
BNA_F
ClientSampleId :
DFTPP