


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
 Data File : BF129845.D
 Acq On : 17 Aug 2022 15:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 18 12:03:10 2022

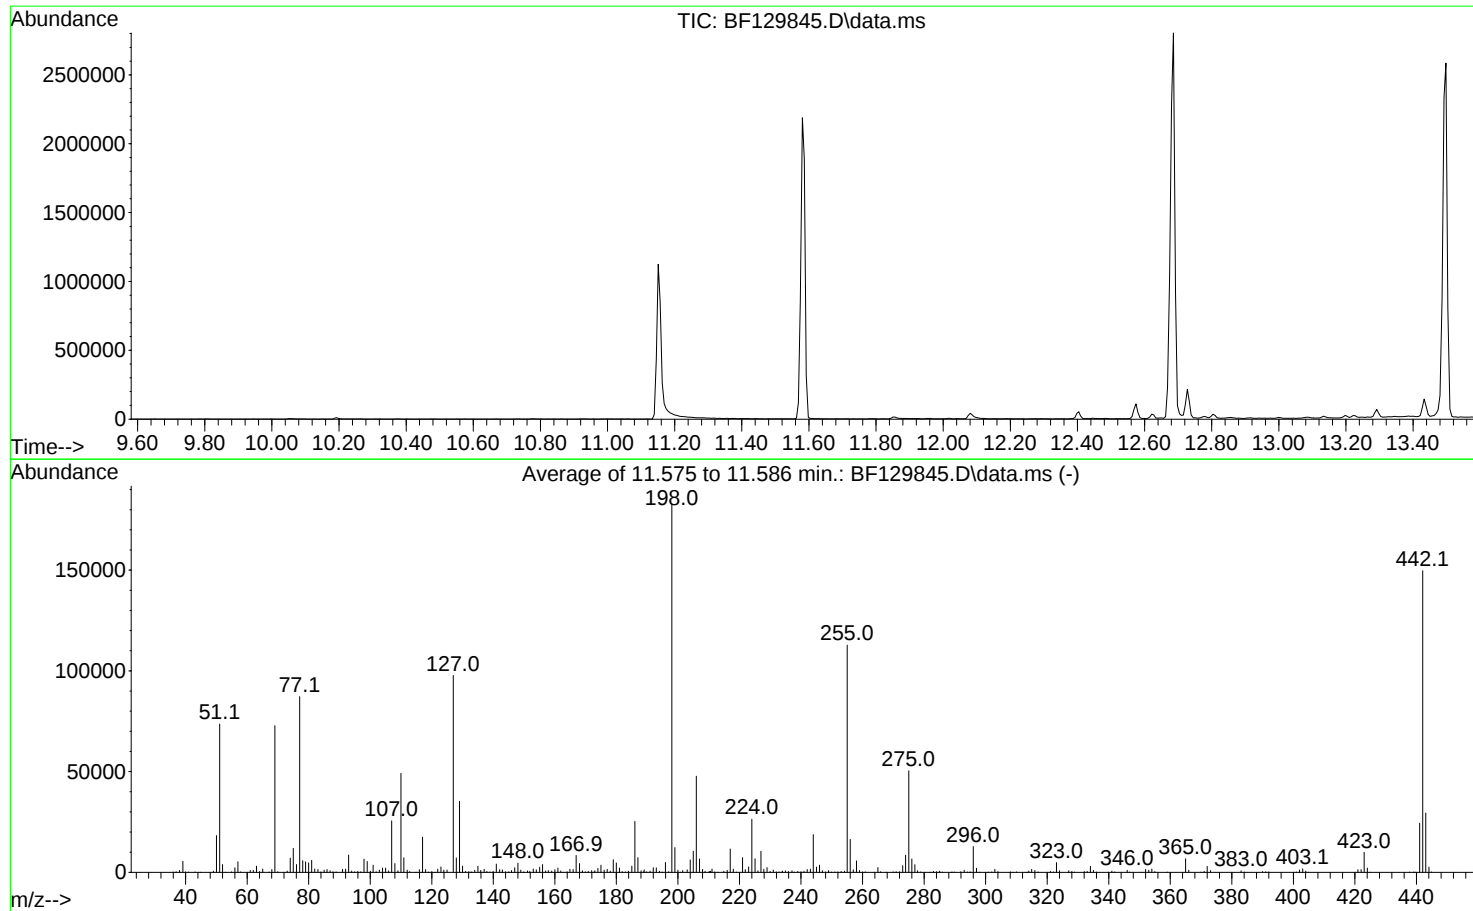




AutoFind: Scans 1579, 1580, 1581; Background Corrected with Scan 1574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	73645	PASS
68	69	0.00	2	1.9	1386	PASS
69	198	0.00	100	39.9	72788	PASS
70	69	0.00	2	0.4	291	PASS
127	198	10	80	53.5	97779	PASS
197	198	0.00	2	0.1	258	PASS
198	198	100	100	100.0	182632	PASS
199	198	5	9	6.7	12292	PASS
275	198	10	60	27.6	50373	PASS
365	198	1	100	3.7	6708	PASS
441	198	0.01	100	13.3	24362	PASS
442	442	50	100	100.0	149688	PASS
443	442	15	24	19.7	29443	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129845.D
Acq On : 17 Aug 2022 15:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:53:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

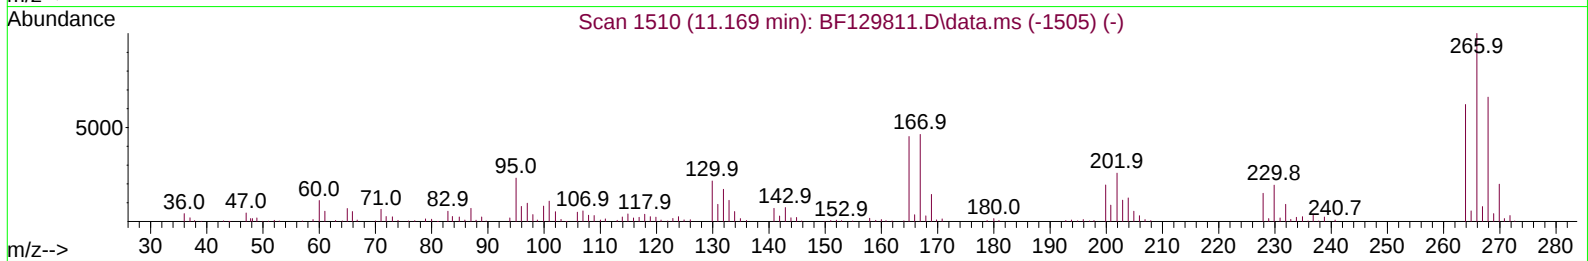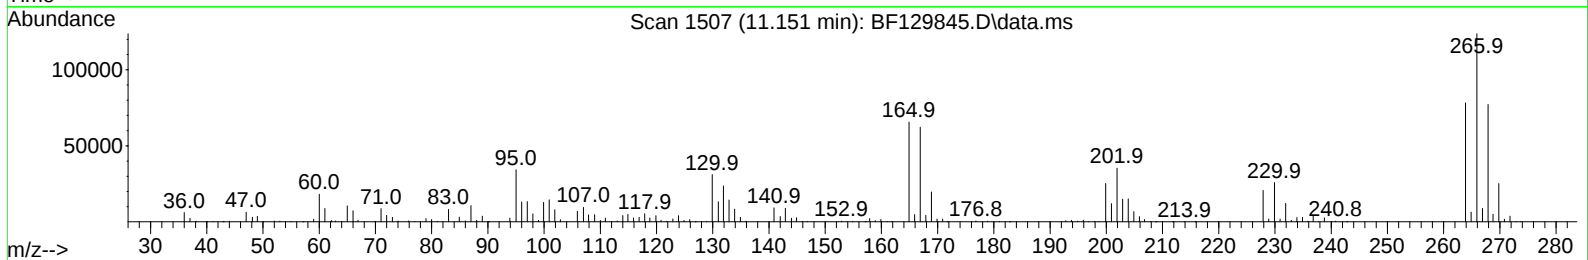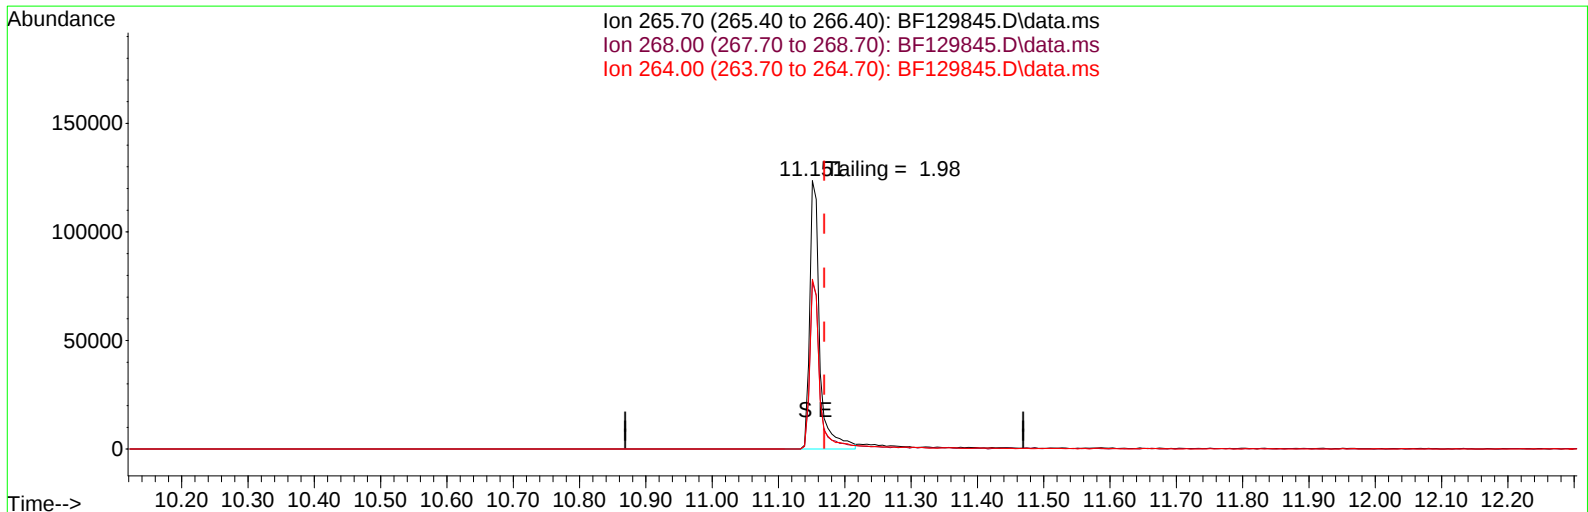

TIC: BF129845.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.018) 395091.80 ng




response 138169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.42
264.00	59.90	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081722\
Data File : BF129845.D
Acq On : 17 Aug 2022 15:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 17:53:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

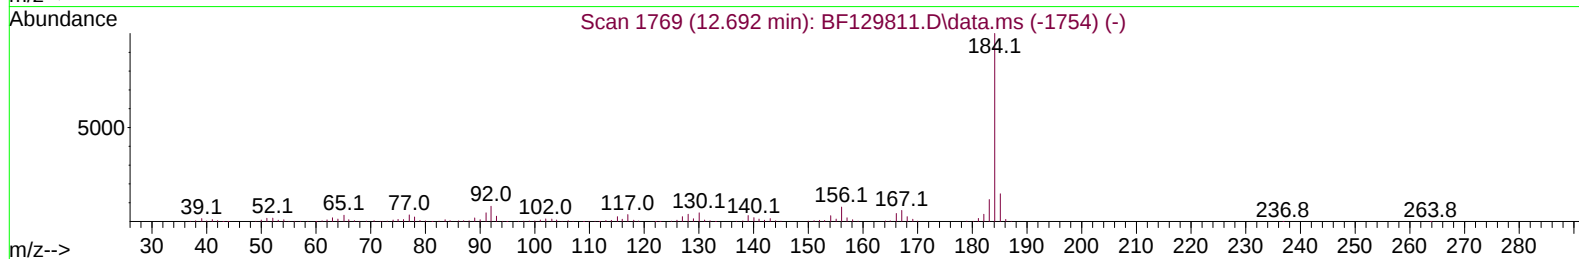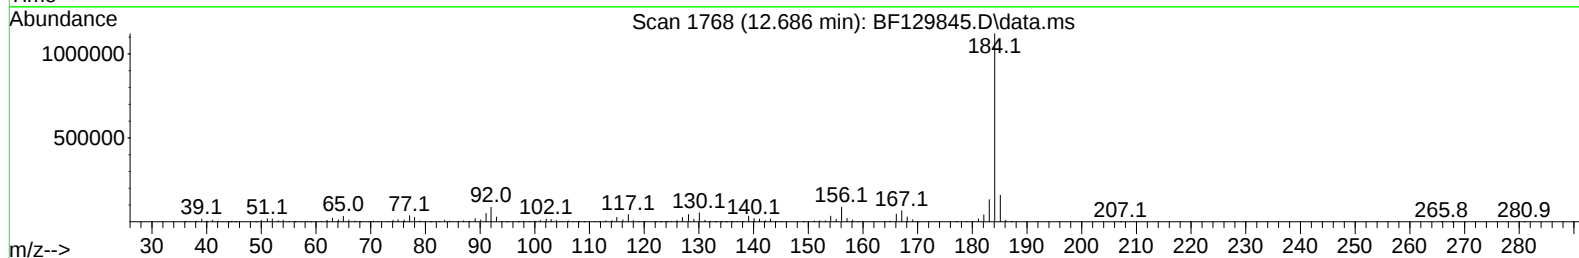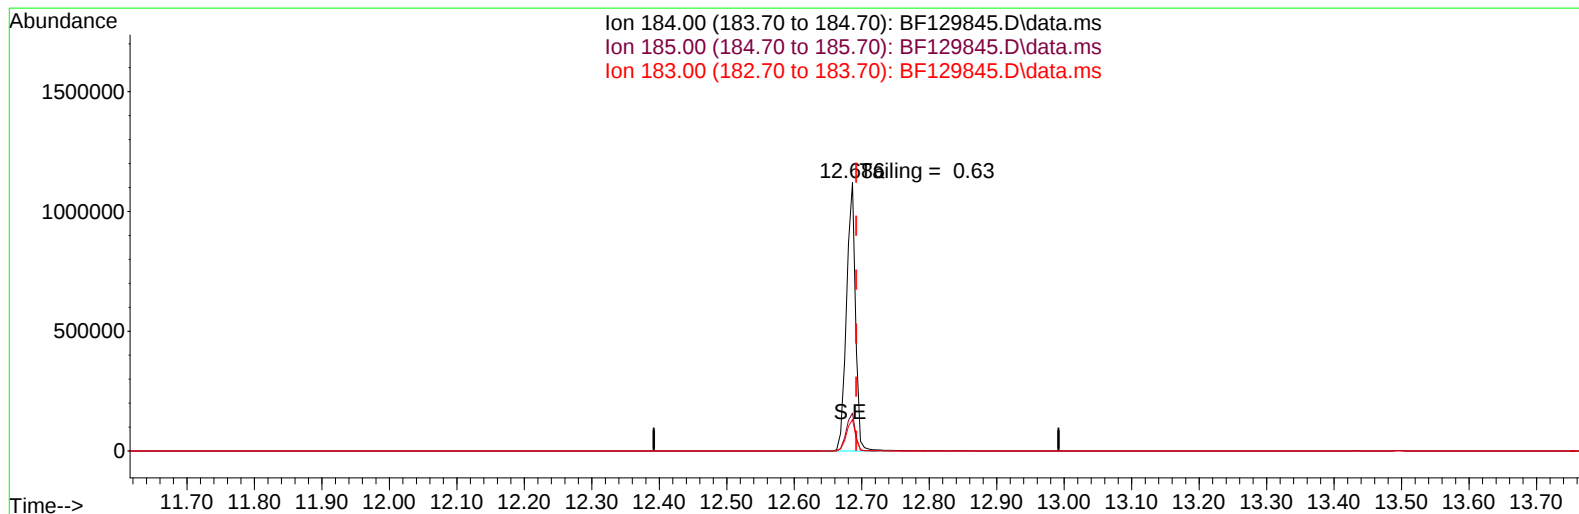

TIC: BF129845.D\data.ms

(77) Benzidine

12.686min (-0.006) 21878.62 ng

response 1040268

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.17
183.00	11.80	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2022	BNA_F	<u>BF129845.D</u>
Compound Name	Response	Retention Time
DDT	457527	13.49
DDD	2867	13.19
DDE	913	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3780	461307	0.82

Instrument :
BNA_F
ClientSampleId :
DFTPP