
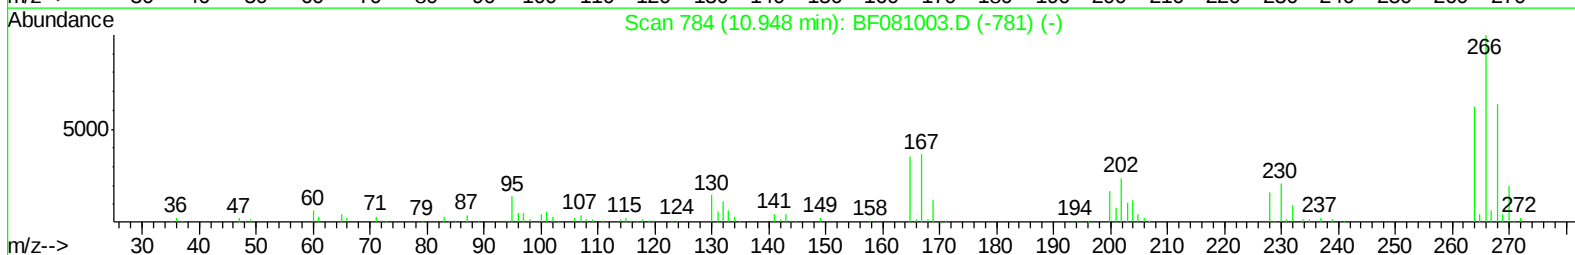
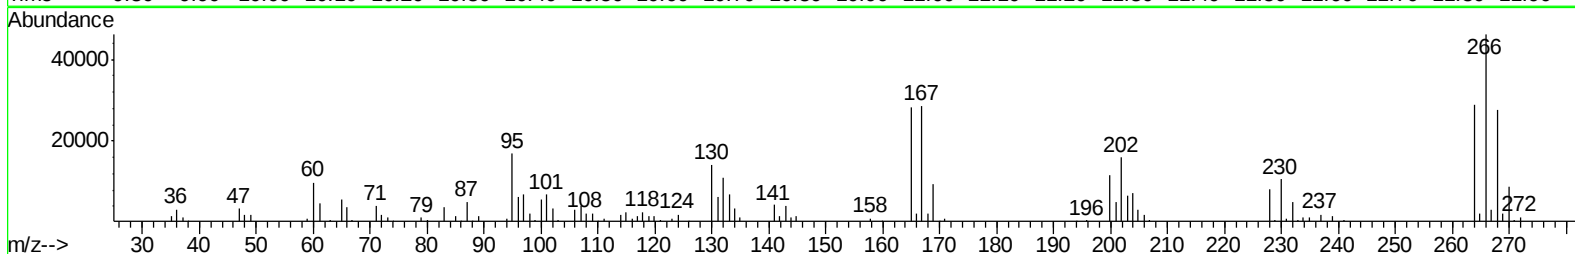


Data Path : Z:\HPCHEM1\BNA_F\Data\BF081815\
Data File : BF081061.D
Acq On : 19 Aug 2015 1:08
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 04:11:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 03:32:45 2015
Response via : Initial Calibration

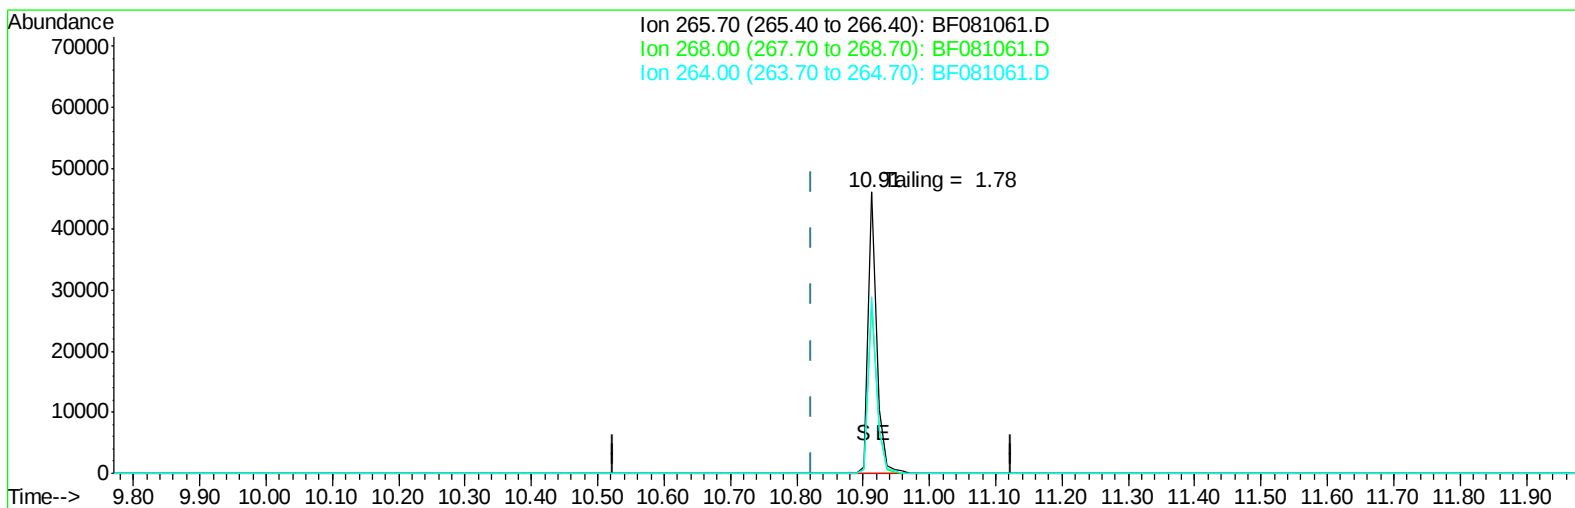

TIC: BF081061.D

(69) Pentachlorophenol (C)




10.913min (+0.090) 0.00ng

response 41324

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	59.97
264.00	63.20	62.72
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF081815\
Data File : BF081061.D
Acq On : 19 Aug 2015 1:08
Operator : UM/IZ
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 04:11:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 03:32:45 2015
Response via : Initial Calibration

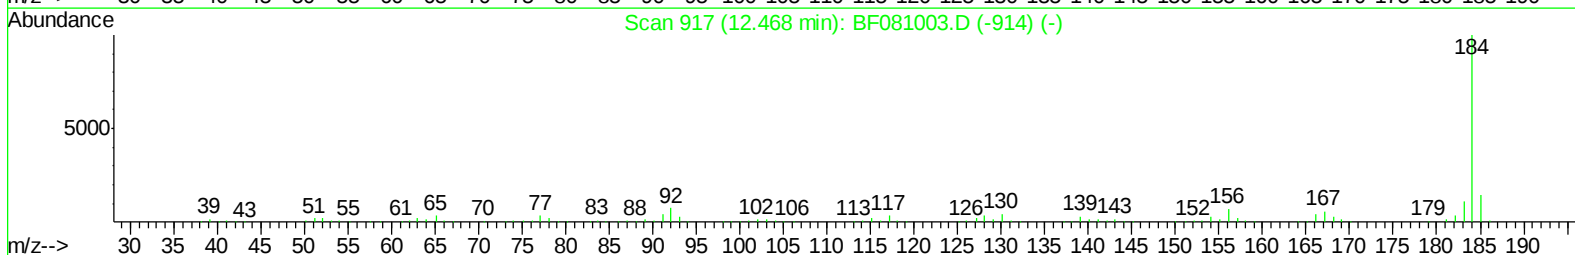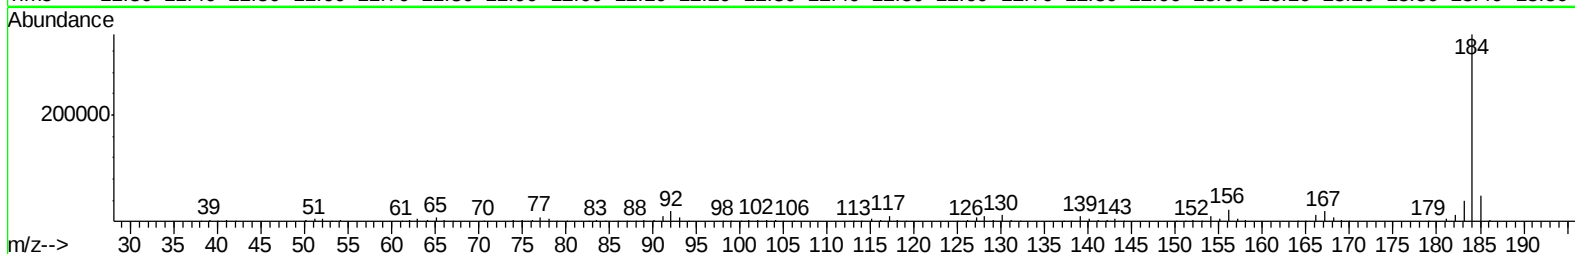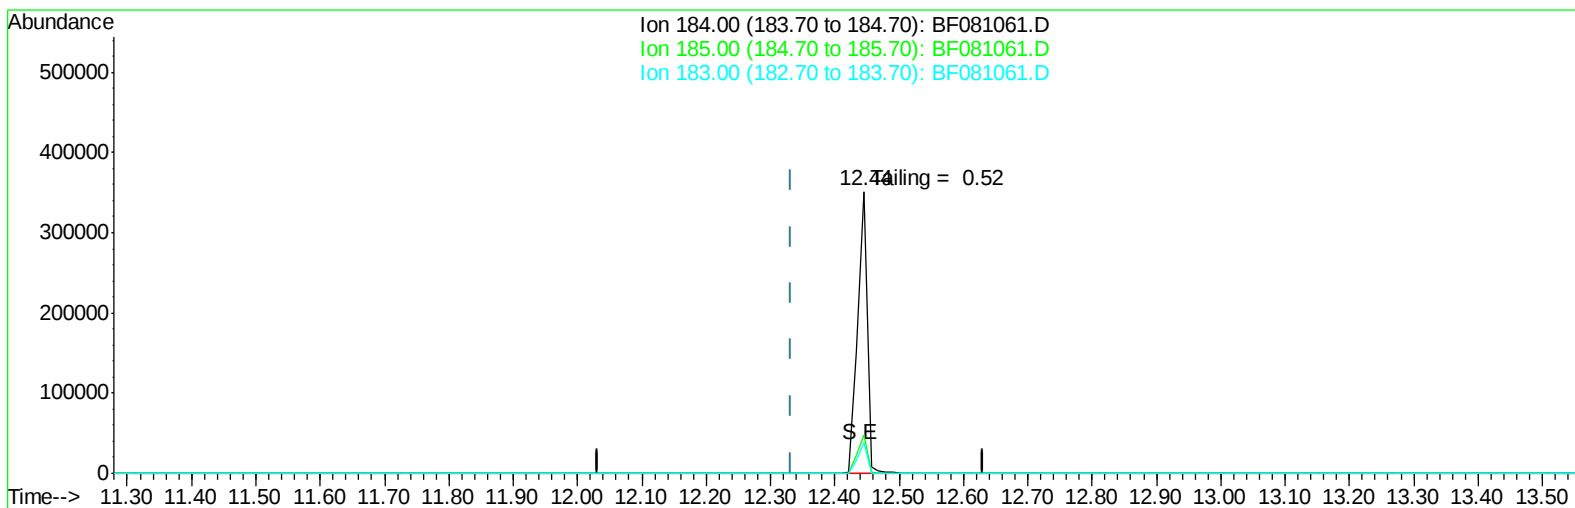

TIC: BF081061.D

(76) Benzidine

12.445min (+0.113) 0.00ng

response 355459

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.84
183.00	11.10	10.90
0.00	0.00	0.00