


Data Path : Z:\HPCHEM1\BNA_F\Data\BF081815\
 Data File : BF081042.D
 Acq On : 18 Aug 2015 14:01
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 17:57:25 2015

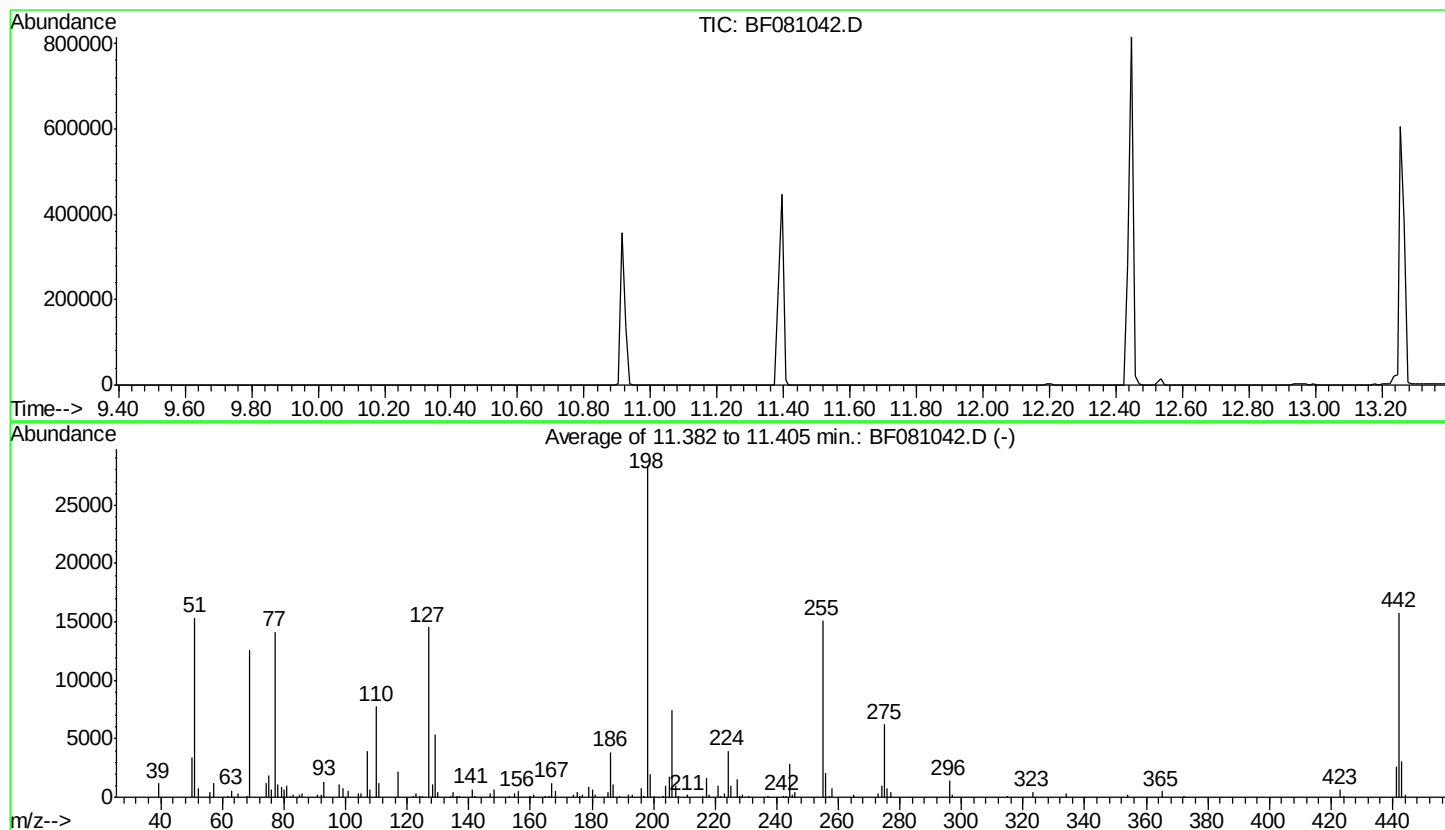

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	15392	PASS
68	69	0.00	2	0.8	103	PASS
69	198	0.00	100	44.5	12637	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	14541	PASS
197	198	0.00	2	0.4	110	PASS
198	198	100	100	100.0	28383	PASS
199	198	5	9	6.9	1953	PASS
275	198	10	60	21.9	6213	PASS
365	198	1	100	1.8	508	PASS
441	442	0.01	24	16.4	2591	PASS
442	198	50	100	55.6	15780	PASS
443	442	15	24	19.6	3090	PASS