


Data Path : Z:\HPCHEM1\BNA_F\Data\BF081815\
 Data File : BF081061.D
 Acq On : 19 Aug 2015 1:08
 Operator : UM/IZ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 17 17:57:25 2015

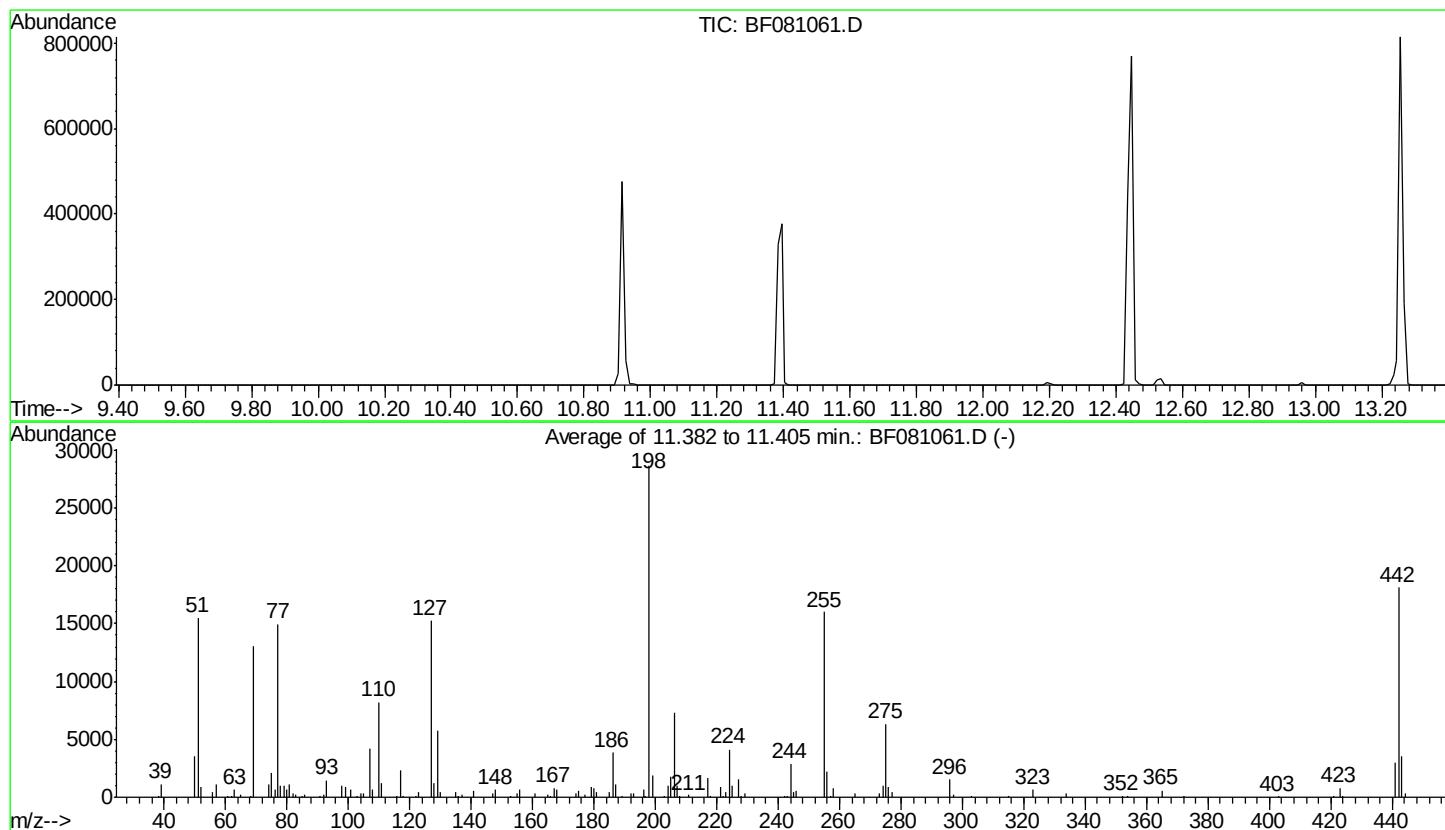

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	15545	PASS
68	69	0.00	2	1.0	132	PASS
69	198	0.00	100	45.4	13005	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	15266	PASS
197	198	0.00	2	0.4	103	PASS
198	198	100	100	100.0	28661	PASS
199	198	5	9	6.4	1841	PASS
275	198	10	60	22.2	6357	PASS
365	198	1	100	2.0	586	PASS
441	442	0.01	24	16.7	3036	PASS
442	198	50	100	63.3	18130	PASS
443	442	15	24	19.7	3572	PASS