
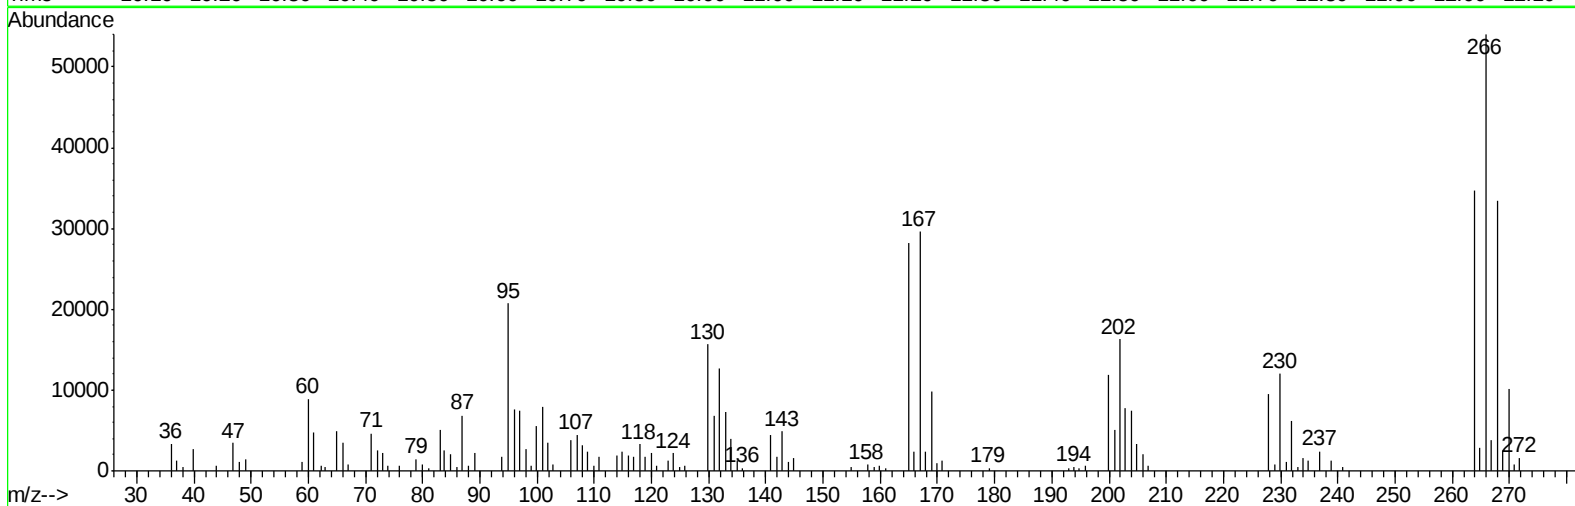


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081817\
Data File : BF097863.D
Acq On : 19 Aug 2017 6:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:29:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

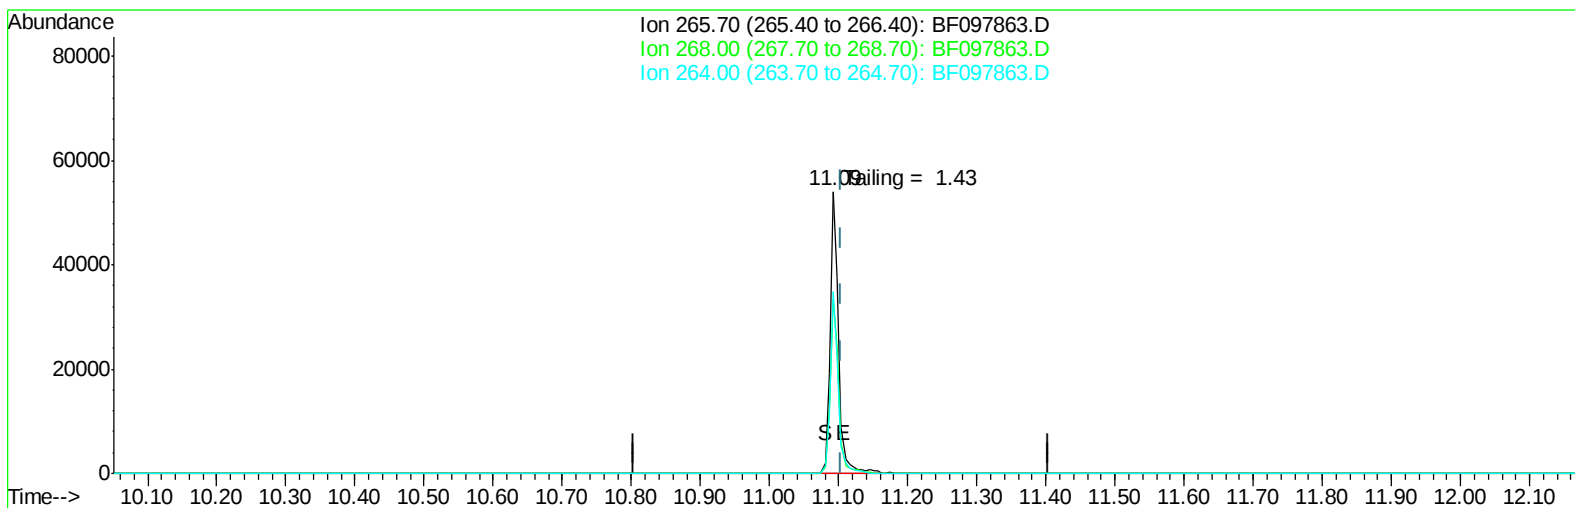

TIC: BF097863.D

(69) Pentachlorophenol (C)



11.092min (-0.012) 15715.53ng m

response 46262

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.01
264.00	64.60	64.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081817\
Data File : BF097863.D
Acq On : 19 Aug 2017 6:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 06:29:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

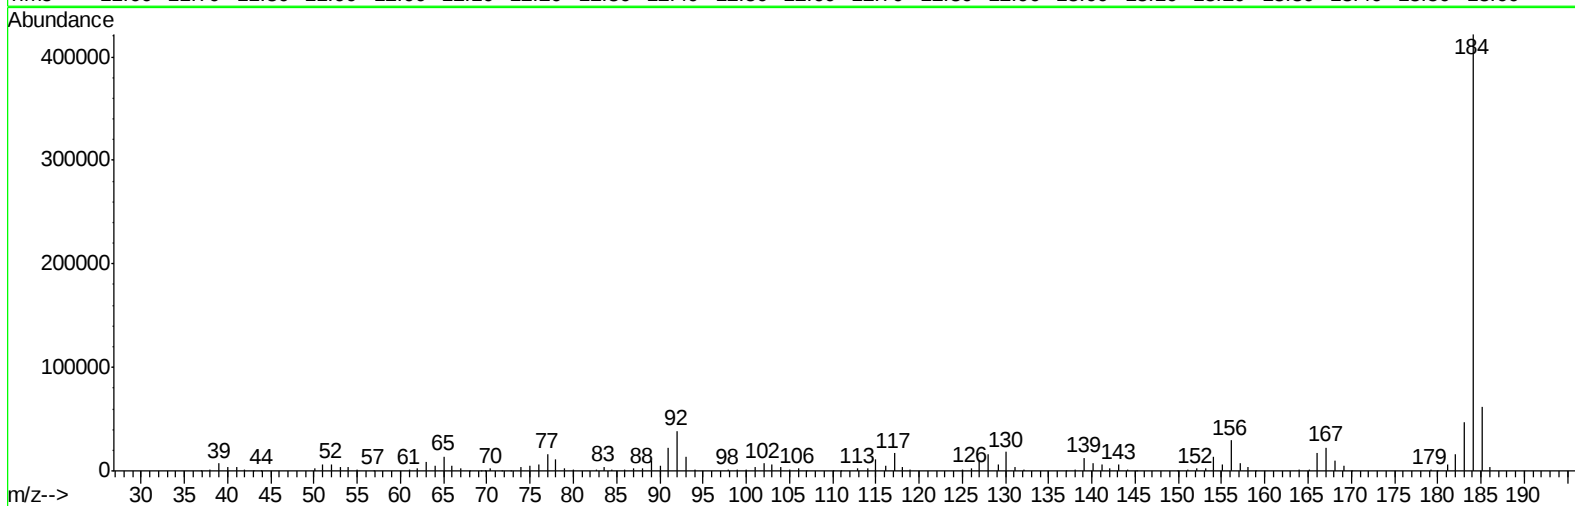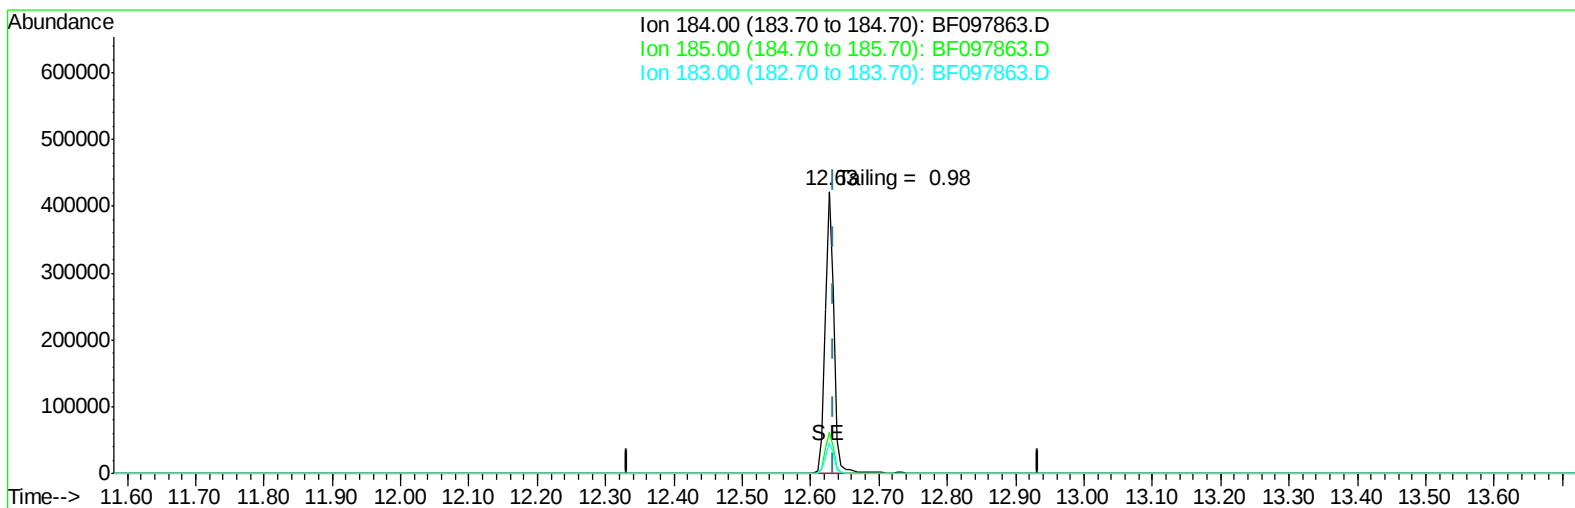

TIC: BF097863.D

(76) Benzidine

12.627min (-0.006) 22740.11ng

response 386965

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.78#
183.00	12.20	11.12
0.00	0.00	0.00