


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081817\
 Data File : BF097837.D
 Acq On : 18 Aug 2017 17:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

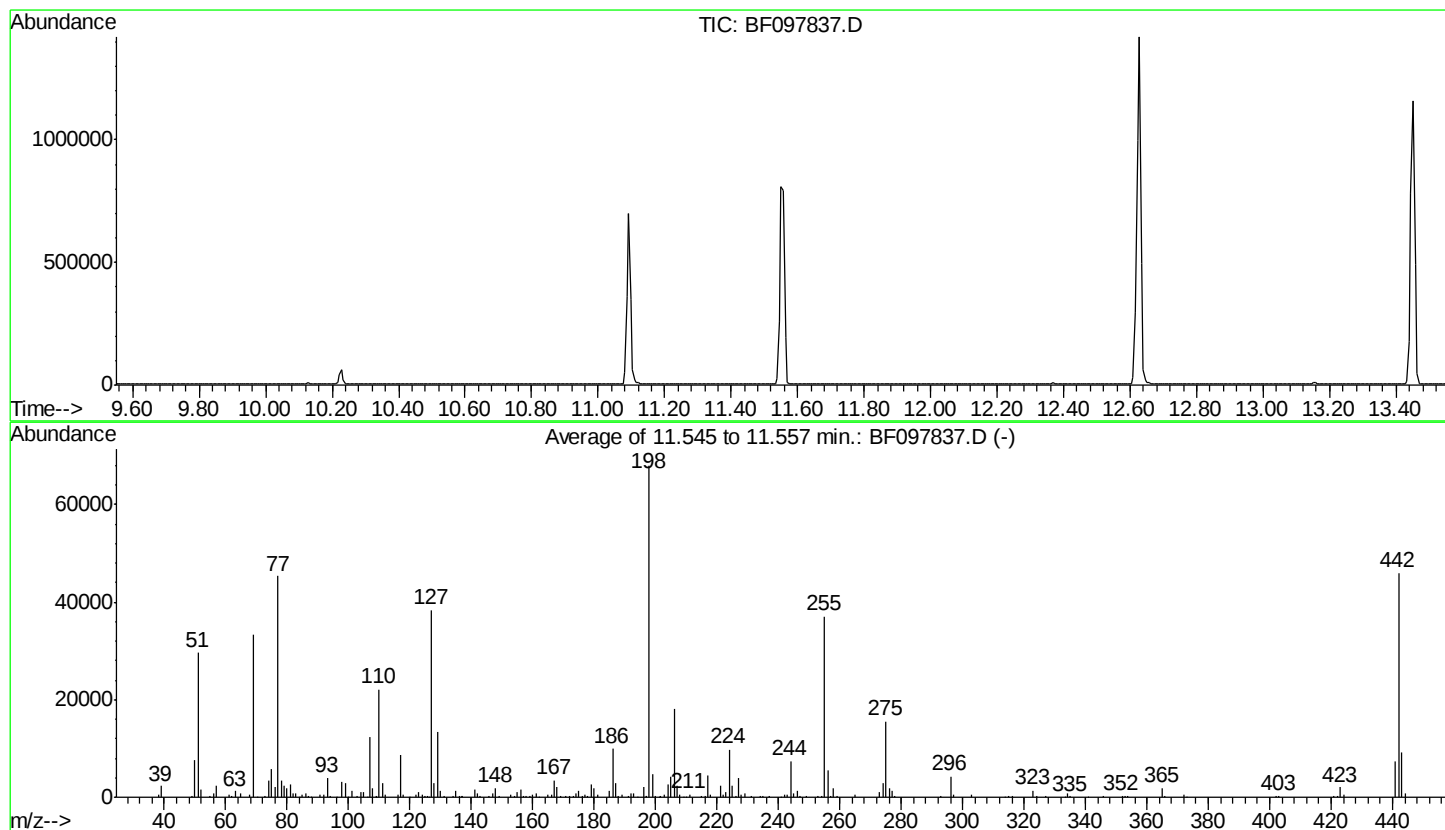

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	29557	PASS
68	69	0.00	2	2.0	656	PASS
69	198	0.00	100	49.0	33338	PASS
70	69	0.00	2	0.4	130	PASS
127	198	10	80	56.4	38336	PASS
197	198	0.00	2	0.5	308	PASS
198	198	100	100	100.0	67984	PASS
199	198	5	9	6.9	4691	PASS
275	198	10	60	22.8	15523	PASS
365	198	1	100	2.8	1929	PASS
441	442	0.01	24	15.9	7315	PASS
442	198	50	100	67.7	46002	PASS
443	442	15	24	19.9	9169	PASS