

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
 Data File : BF129874.D
 Acq On : 18 Aug 2022 14:12
 Operator : CG\JU
 Sample : N4189-09RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB16RE

Quant Time: Aug 18 14:41:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 18 12:03:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.793	152	128557	20.000	ng	0.00
21) Naphthalene-d8	8.075	136	520840	20.000	ng	0.00
39) Acenaphthene-d10	9.828	164	274433	20.000	ng	0.00
64) Phenanthrene-d10	11.322	188	454836	20.000	ng	0.00
76) Chrysene-d12	13.969	240	220119	20.000	ng	0.00
86) Perylene-d12	15.433	264	249928	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	326576	42.060	ng	0.00
7) Phenol-d6	6.446	99	407661	41.926	ng	0.00
23) Nitrobenzene-d5	7.357	82	250594	25.756	ng	-0.01
42) 2,4,6-Tribromophenol	10.628	330	95032	34.503	ng	0.00
45) 2-Fluorobiphenyl	9.145	172	481896	26.670	ng	0.00
79) Terphenyl-d14	12.904	244	408893	30.909	ng	0.00
Target Compounds						
					Qvalue	
9) Benzaldehyde	6.446	77	533	Below Cal	#	1
19) n-Nitroso-di-n-propyla...	7.357	70	32146	5.230 ng	#	77
25) Isophorone	7.357	82	250591	14.964 ng	#	65
32) Benzoic acid	8.069	122	60	2.174 ng	#	1
51) 2,6-Dinitrotoluene	9.828	165	35075	8.219 ng	#	23
57) 2,4-Dinitrotoluene	9.828	165	35075	6.331 ng	#	18
77) Benzidine	12.904	184	5401	Below Cal	#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129874.D
Acq On : 18 Aug 2022 14:12
Operator : CG\JU
Sample : N4189-09RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB16RE

Quant Time: Aug 18 14:41:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration




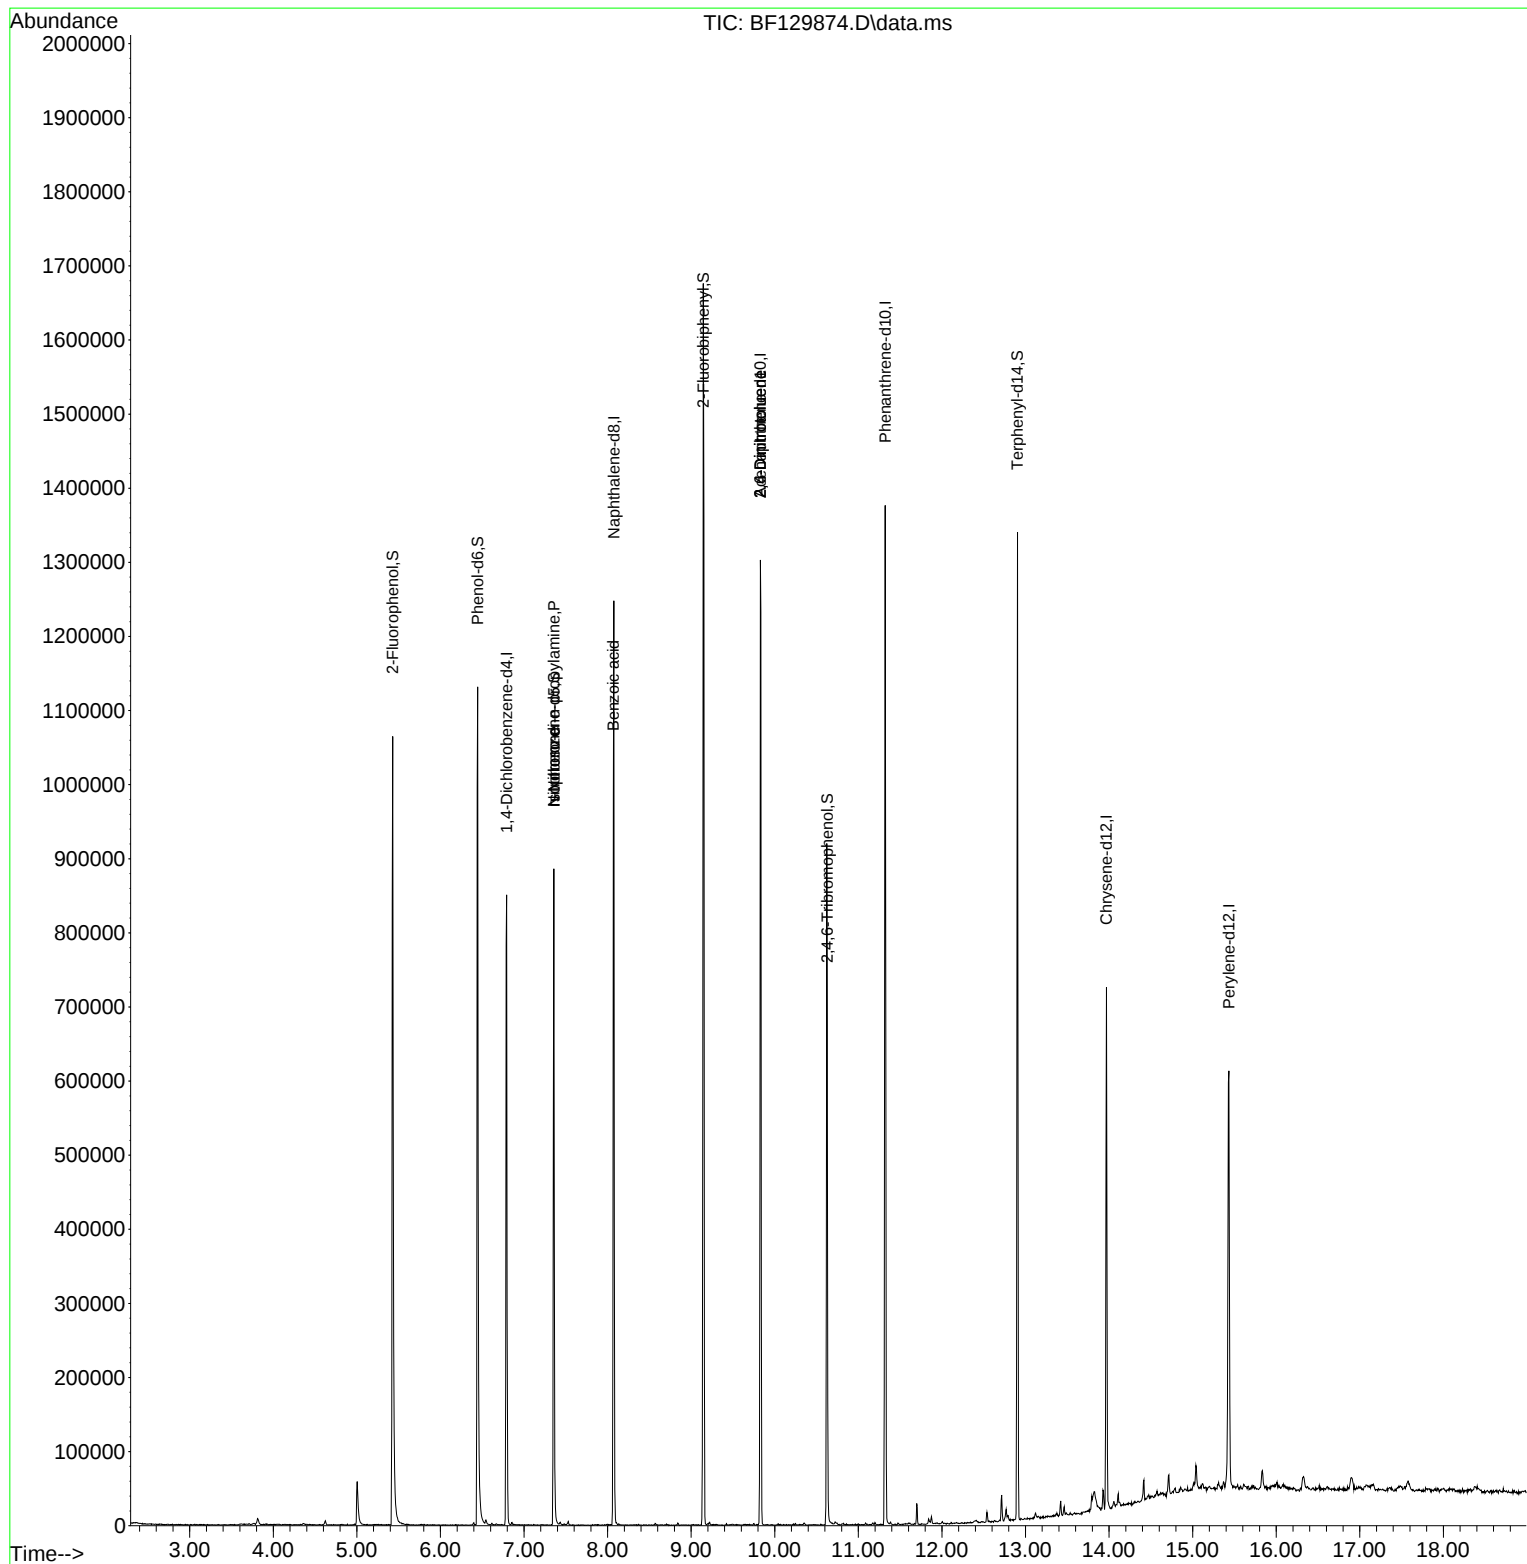




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.793 min Scan# 70
Delta R.T. 0.001 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE

Tgt Ion:152 Resp: 128557
Ion Ratio Lower Upper
152 100
150 153.8 126.9 190.3
115 63.5 53.4 80.0

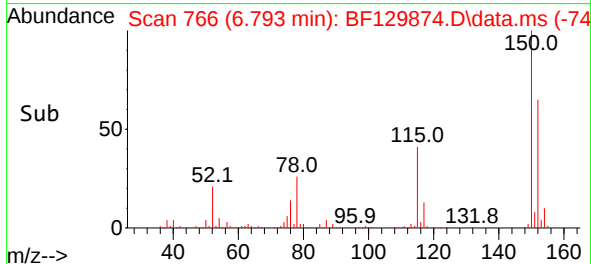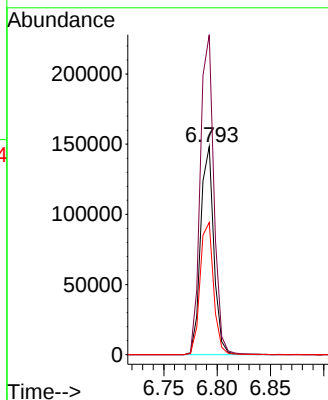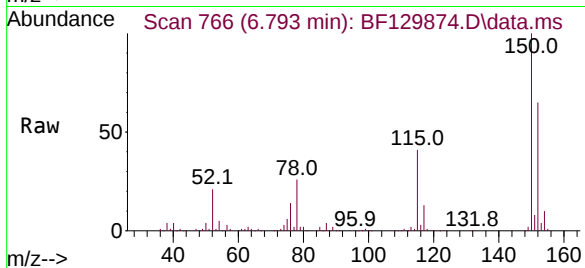

#5
2-Fluorophenol
Concen: 42.060 ng
RT: 5.428 min Scan# 534
Delta R.T. 0.000 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion:112 Resp: 326576
Ion Ratio Lower Upper
112 100
64 58.2 47.6 71.4
63 30.3 24.6 37.0



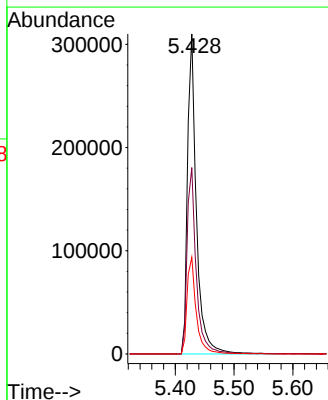
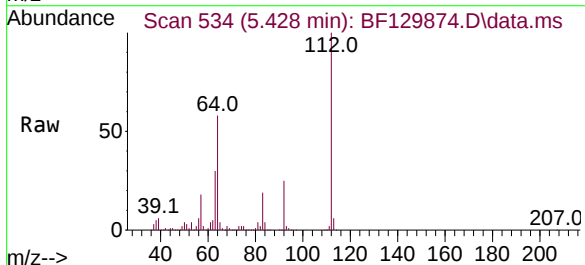




#7
Phenol-d6
Concen: 41.926 ng
RT: 6.446 min Scan# 707
Delta R.T. -0.006 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE

Tgt Ion: 99 Resp: 407661
Ion Ratio Lower Upper
99 100
42 17.8 15.0 22.4
71 35.4 28.8 43.2

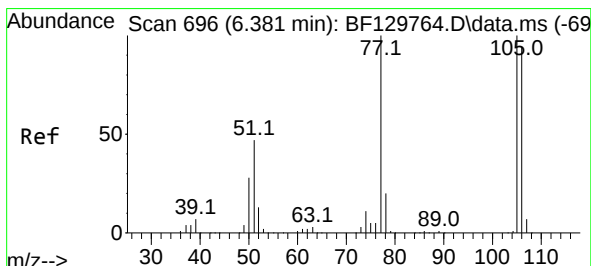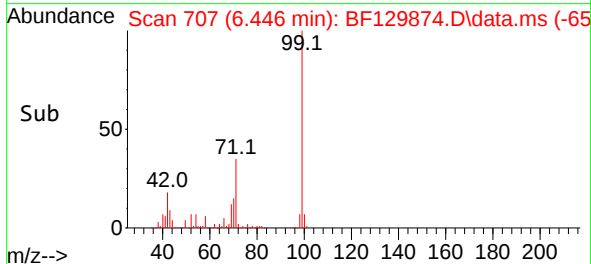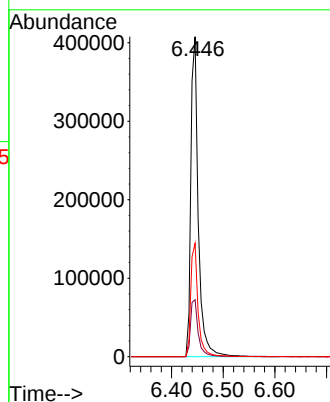

#9
Benzaldehyde
Concen: Below Cal
RT: 6.446 min Scan# 707
Delta R.T. 0.094 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion: 77 Resp: 533
Ion Ratio Lower Upper
77 100
105 0.0 80.3 120.3#
106 0.0 74.3 114.3#


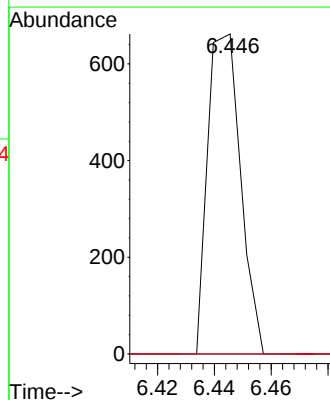





#19
n-Nitroso-di-n-propylamine
Concen: 5.230 ng
RT: 7.357 min Scan# 80
Delta R.T. 0.147 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE

Tgt Ion: 70 Resp: 32146
Ion Ratio Lower Upper
70 100
42 47.9 47.6 71.4
101 0.0 8.1 12.1#
130 1.7 17.2 25.8#

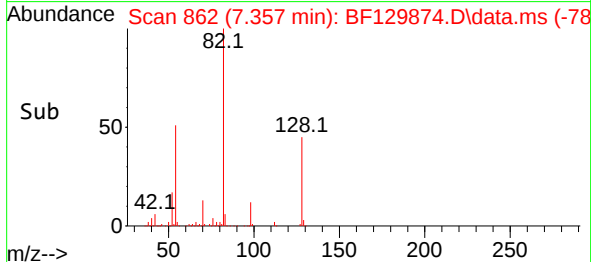

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.075 min Scan# 984
Delta R.T. -0.006 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion:136 Resp: 520840
Ion Ratio Lower Upper
136 100
137 10.8 8.4 12.6
54 7.3 6.2 9.2
68 5.2 4.2 6.4


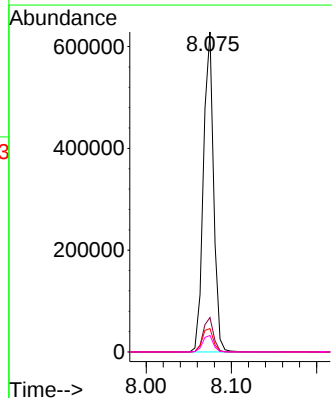
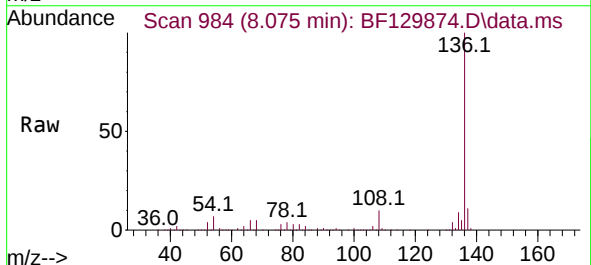




#23
Nitrobenzene-d5
Concen: 25.756 ng
RT: 7.357 min Scan# 80
Delta R.T. -0.012 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE

Tgt Ion: 82 Resp: 250594
Ion Ratio Lower Upper
82 100
128 44.5 36.1 54.1
54 50.7 40.0 60.0

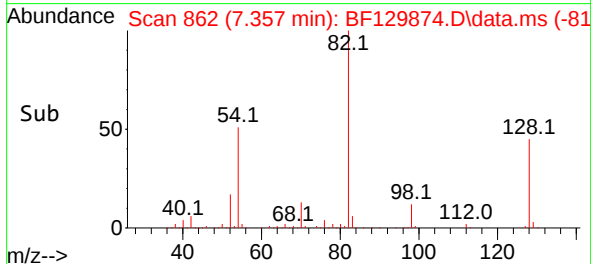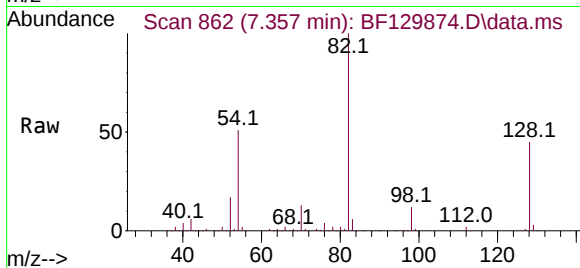

#25
Isophorone
Concen: 14.964 ng
RT: 7.357 min Scan# 862
Delta R.T. -0.264 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion: 82 Resp: 250591
Ion Ratio Lower Upper
82 100
95 0.0 5.9 8.9#
138 0.0 14.6 21.8#




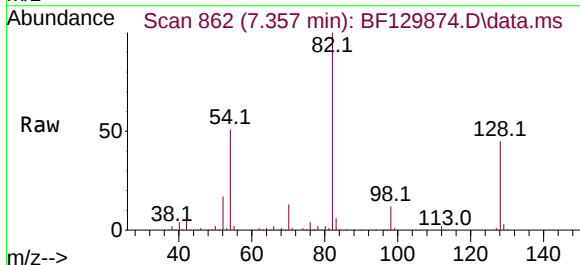




#32
Benzoic acid
Concen: 2.174 ng
RT: 8.069 min Scan# 91
Delta R.T. 0.183 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE


Tgt Ion:122 Resp: 60
Ion Ratio Lower Upper
122 100
105 275.1 99.9 139.9#
77 968.0 65.9 105.9#

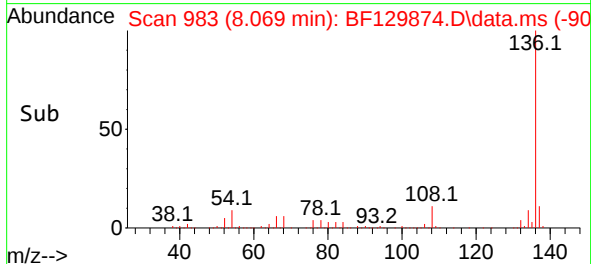

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.828 min Scan# 1282
Delta R.T. -0.006 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion:164 Resp: 274433
Ion Ratio Lower Upper
164 100
162 104.8 82.0 123.0
160 44.8 35.4 53.0

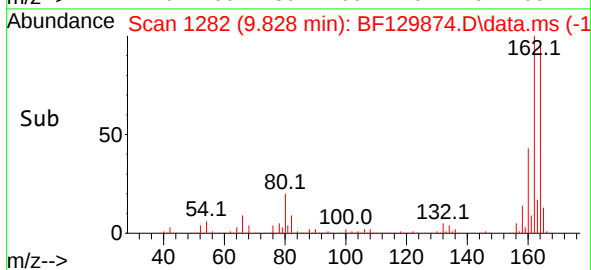

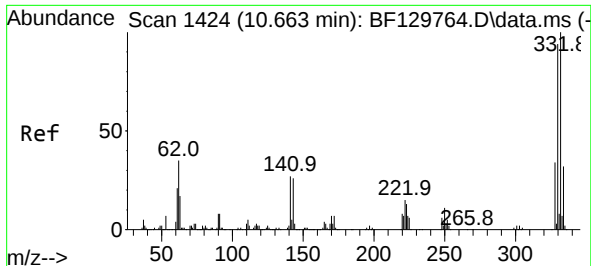

#42

2,4,6-Tribromophenol

Concen: 34.503 ng

RT: 10.628 min Scan# 1424

Delta R.T. 0.000 min

Lab File: BF129874.D

Acq: 18 Aug 2022 14:12

Instrument :

BNA_F

ClientSampleId :

SB16RE




Tgt Ion:330 Resp: 95032

Ion Ratio Lower Upper

330 100

332 105.4 82.6 124.0

141 36.8 27.6 41.4

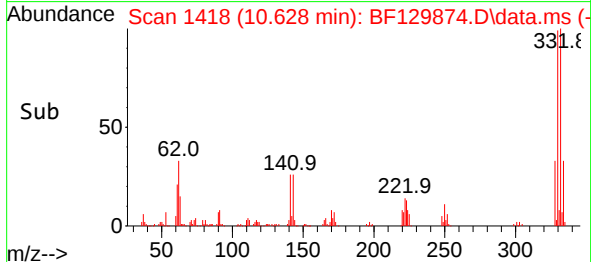

#45

2-Fluorobiphenyl

Concen: 26.670 ng

RT: 9.145 min Scan# 1166

Delta R.T. -0.006 min

Lab File: BF129874.D

Acq: 18 Aug 2022 14:12




Tgt Ion:172 Resp: 481896

Ion Ratio Lower Upper

172 100

171 35.5 28.4 42.6

170 23.0 19.1 28.7



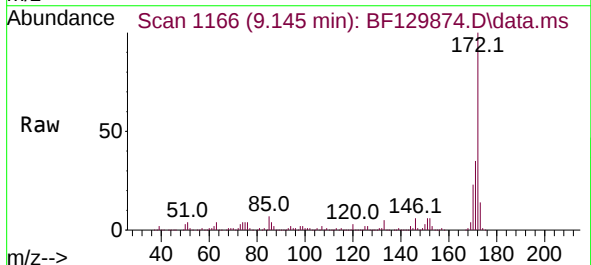




#51
2,6-Dinitrotoluene
Concen: 8.219 ng
RT: 9.828 min Scan# 11
Delta R.T. 0.200 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE

Tgt Ion:165 Resp: 35075
Ion Ratio Lower Upper
165 100
63 1.4 47.8 71.8#
89 1.8 47.2 70.8#

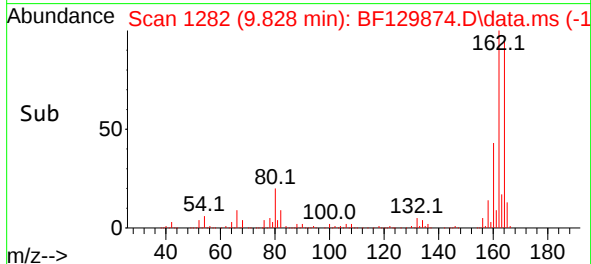

#57
2,4-Dinitrotoluene
Concen: 6.331 ng
RT: 9.828 min Scan# 1282
Delta R.T. -0.212 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion:165 Resp: 35075
Ion Ratio Lower Upper
165 100
63 1.4 48.4 72.6#
89 1.8 62.3 93.5#
182 0.0 2.1 3.1#


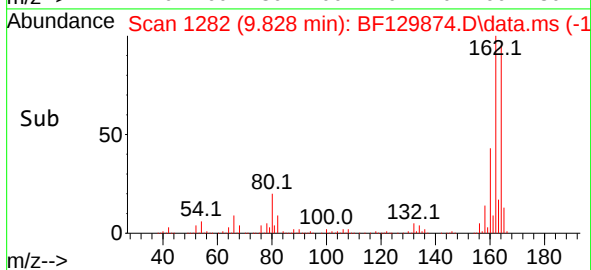






#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.322 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE


Tgt Ion:188 Resp: 454836
Ion Ratio Lower Upper
188 100
94 8.9 7.4 11.2
80 10.2 7.9 11.9

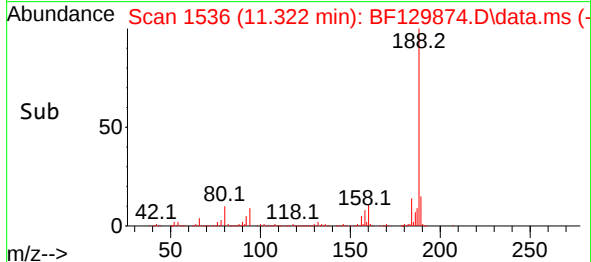

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.969 min Scan# 1986
Delta R.T. -0.006 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12

Tgt Ion:240 Resp: 220119
Ion Ratio Lower Upper
240 100
120 11.7 9.2 13.8
236 25.6 20.7 31.1


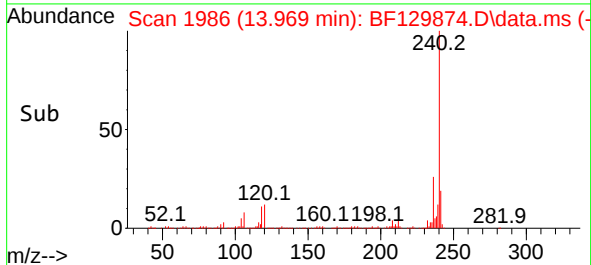






#77
Benzidine
Concen: Below Cal
RT: 12.904 min Scan# 1805
Delta R.T. 0.241 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12




Instrument :
BNA_F
ClientSampleId :
SB16RE


Tgt Ion:184 Resp: 5401
Ion Ratio Lower Upper
184 100
185 19.1 11.4 17.2#
183 7.6 9.4 14.2#

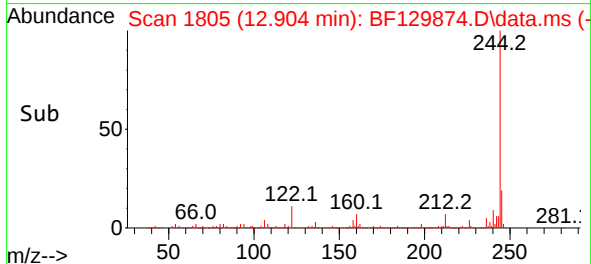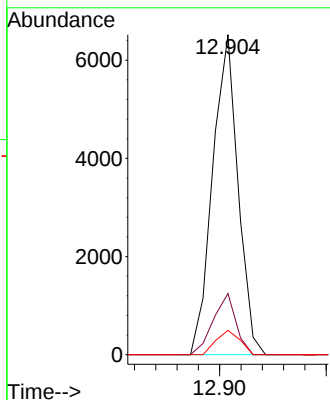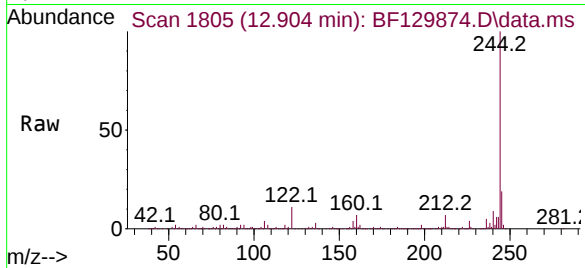

#79
Terphenyl-d14
Concen: 30.909 ng
RT: 12.904 min Scan# 1805
Delta R.T. -0.006 min
Lab File: BF129874.D
Acq: 18 Aug 2022 14:12


Tgt Ion:244 Resp: 408893
Ion Ratio Lower Upper
244 100
212 6.7 5.9 8.9
122 11.0 9.9 14.9

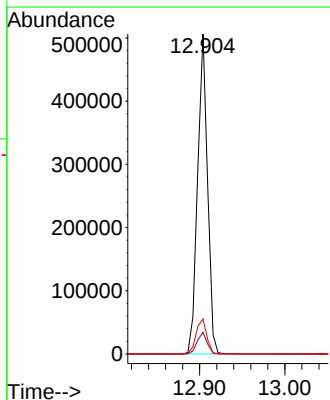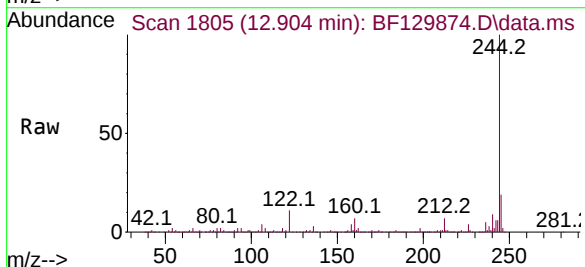

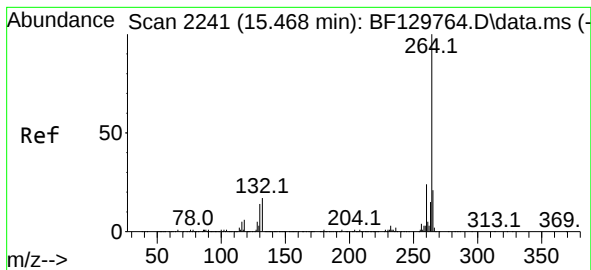

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.433 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BF129874.D
 Acq: 18 Aug 2022 14:12

Instrument :
 BNA_F
 ClientSampleId :
 SB16RE

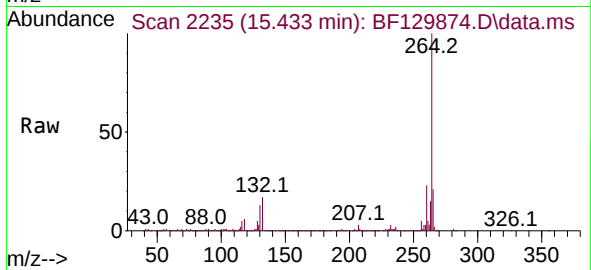

Tgt Ion:264 Resp: 249928
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.1 28.7
 265 20.9 16.7 25.1

