
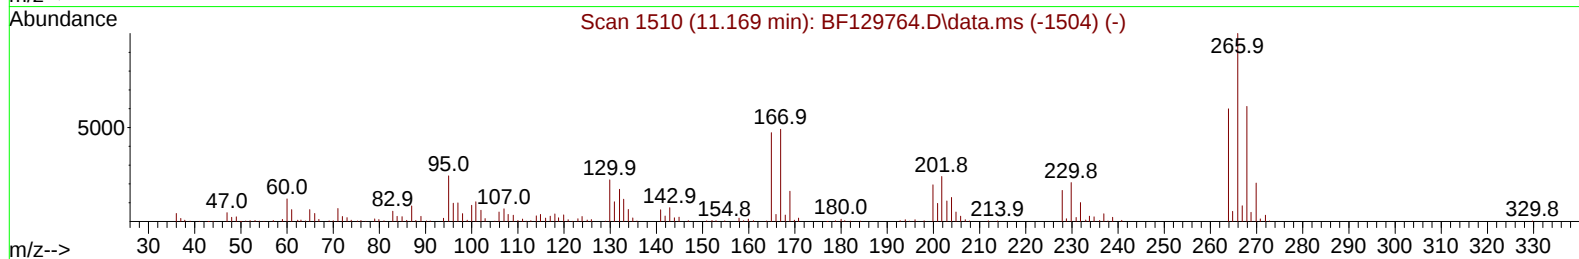
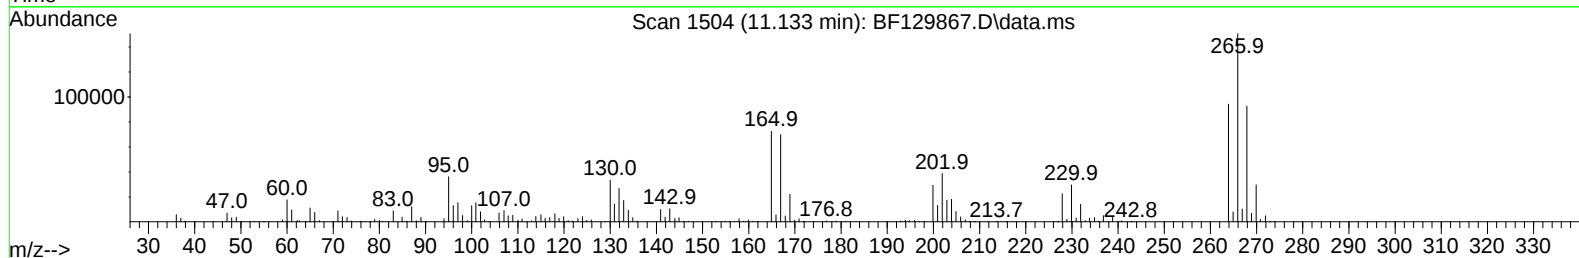


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129867.D
Acq On : 18 Aug 2022 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 07:15:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration

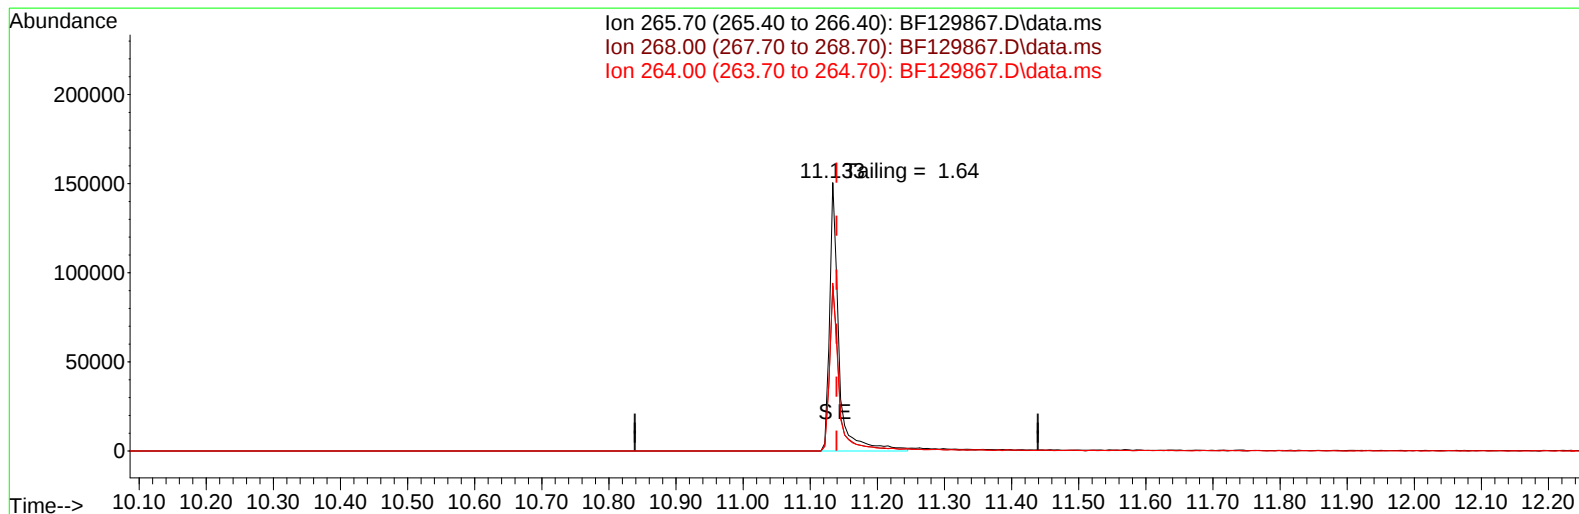

TIC: BF129867.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.006) 83969.20 ng

response 145453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.47
264.00	59.90	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
 Data File : BF129867.D
 Acq On : 18 Aug 2022 10:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 07:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 18 12:03:10 2022
 Response via : Initial Calibration

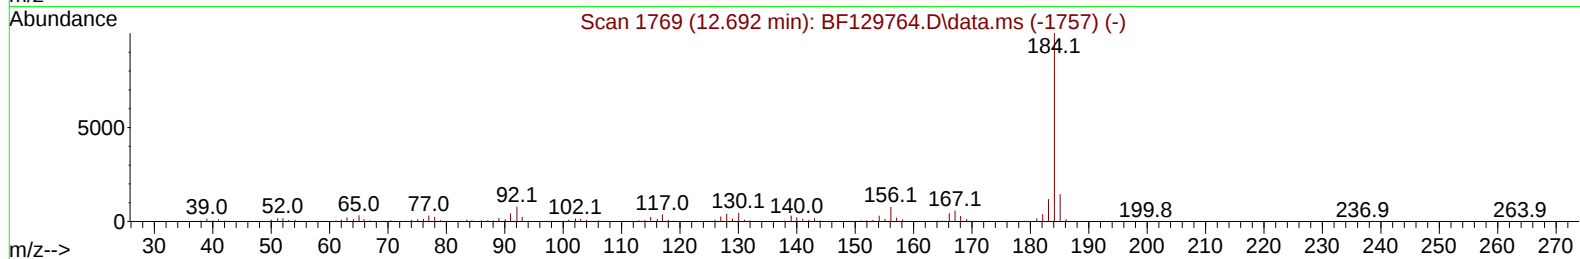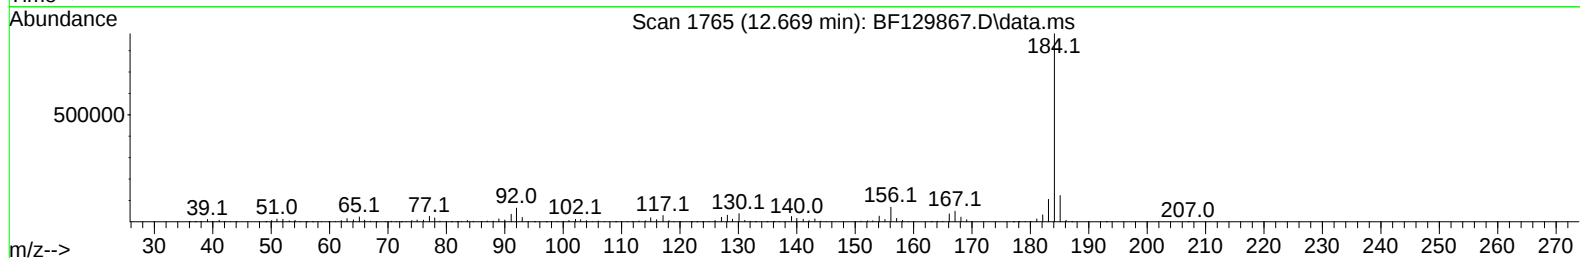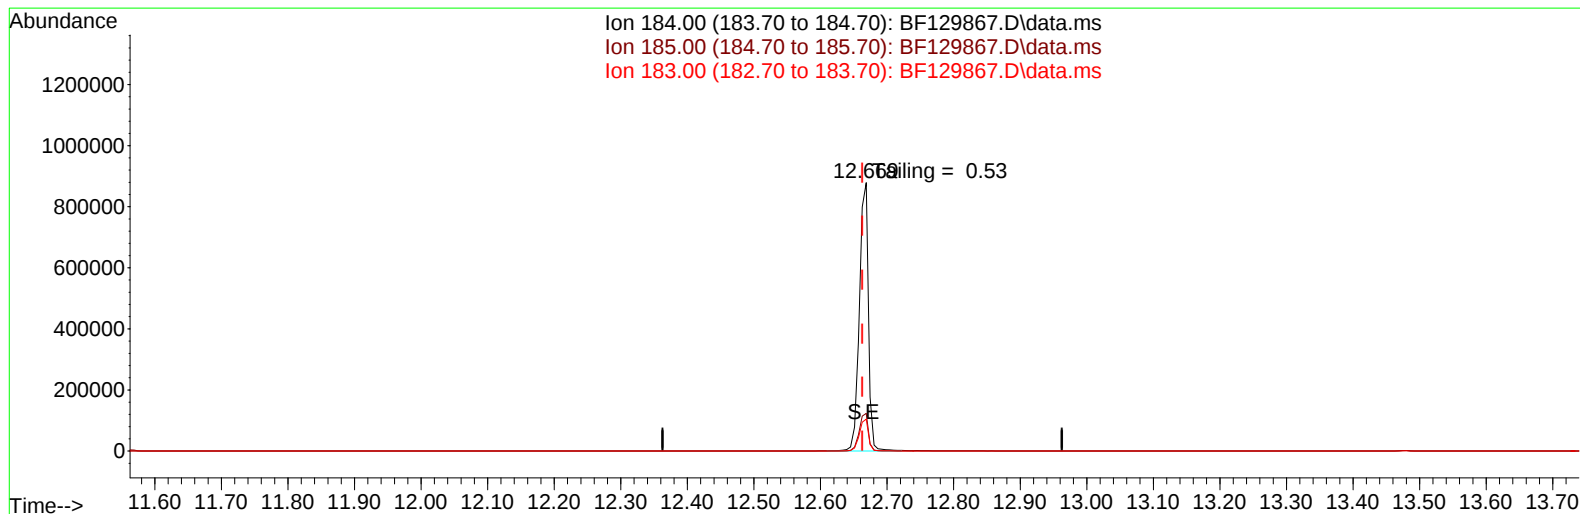

TIC: BF129867.D\data.ms

(77) Benzidine**12.669min (+ 0.006) 150382.43 ng****response 836332**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.01
183.00	11.80	11.90
0.00	0.00	0.00