
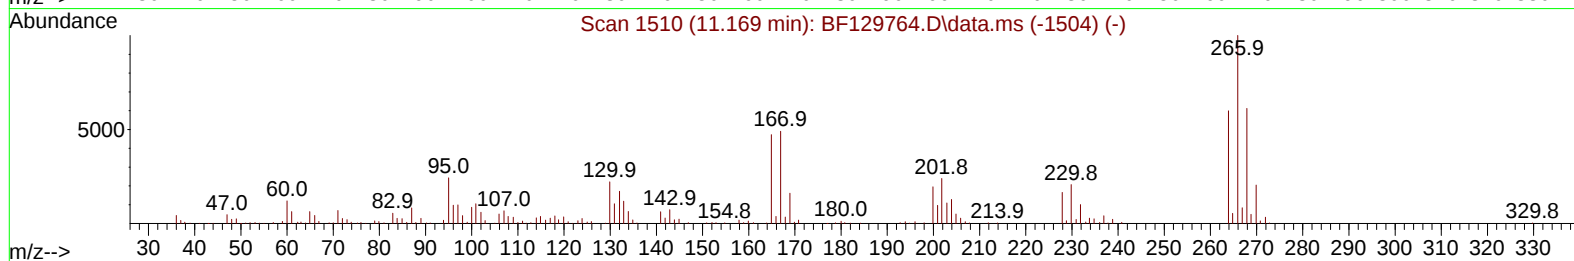
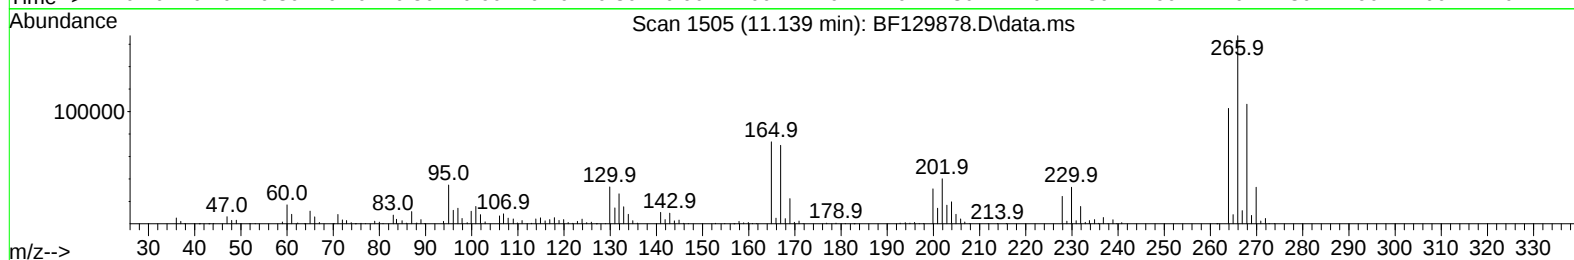


Quant Time: Aug 19 05:02:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration

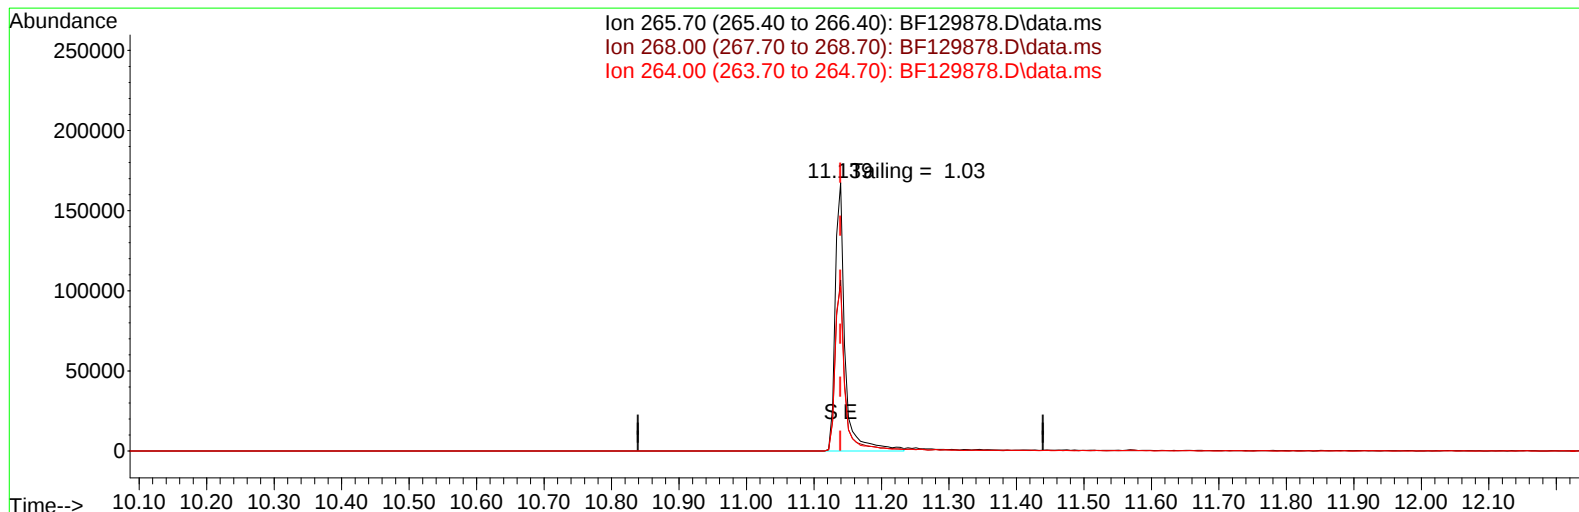

TIC: BF129878.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 496402.47 ng

response **169562**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.61
264.00	59.90	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129878.D
Acq On : 18 Aug 2022 16:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 05:02:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration

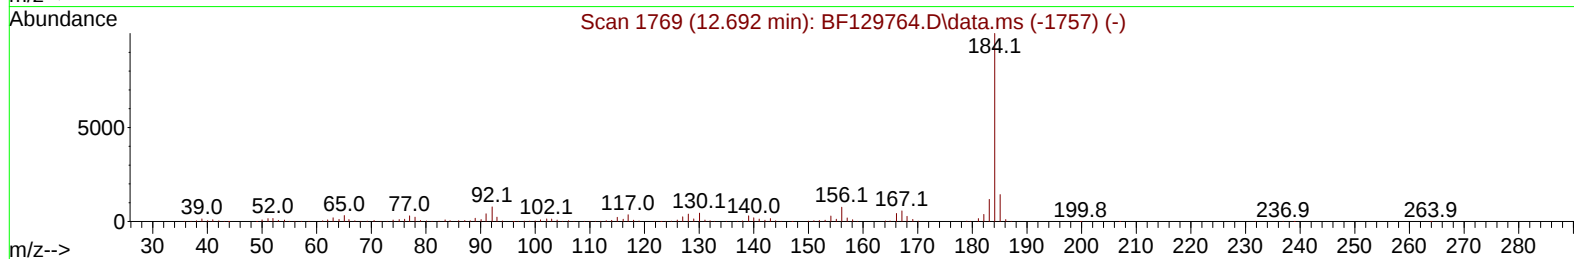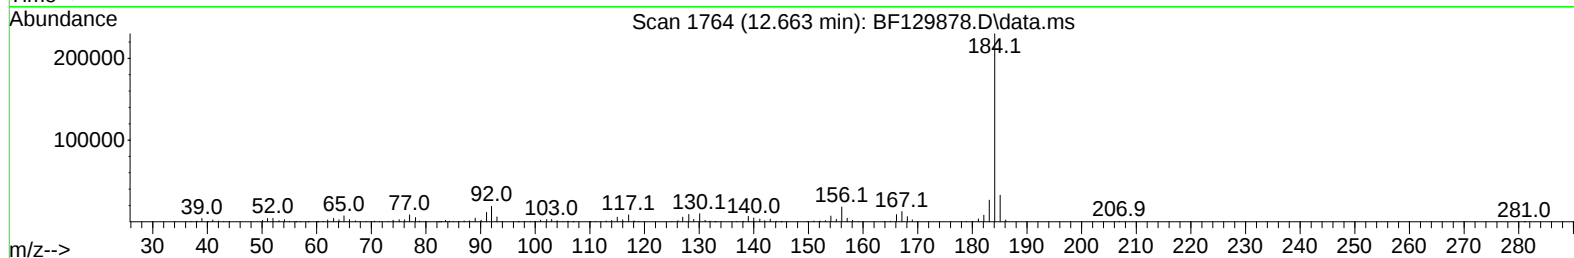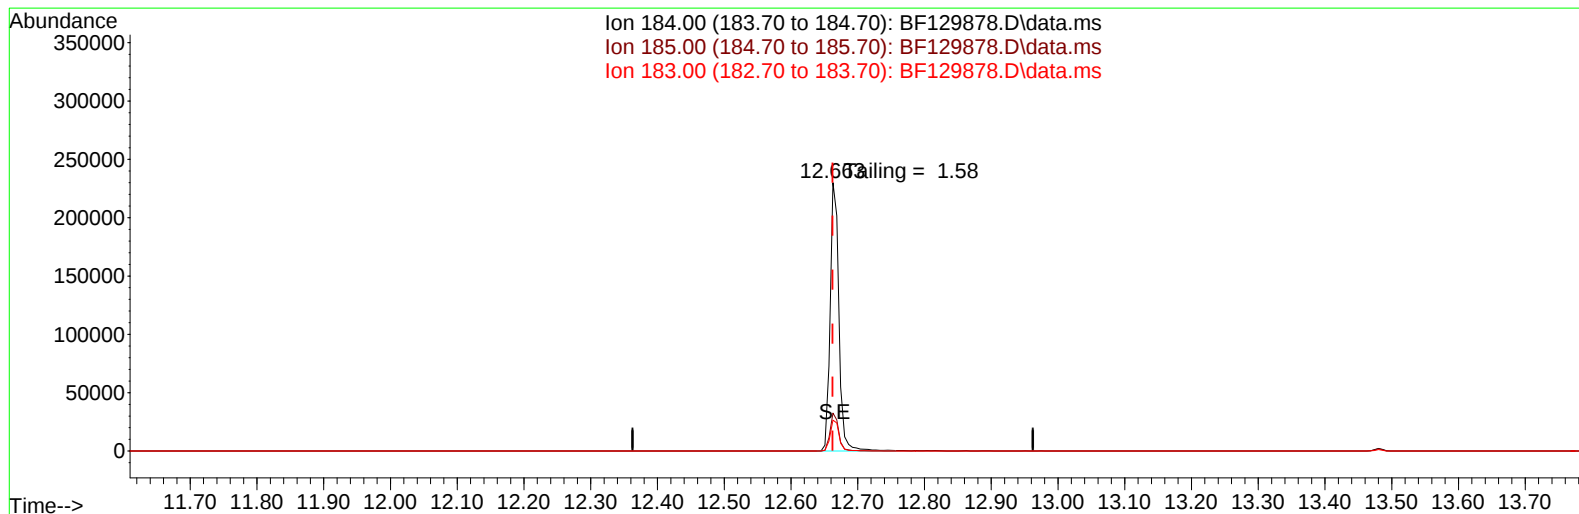

TIC: BF129878.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 65799.48 ng

response 211502

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.16
183.00	11.80	11.53
0.00	0.00	0.00