

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
 Data File : BF129869.D
 Acq On : 18 Aug 2022 11:22
 Operator : CG\JU
 Sample : PB146986BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146986BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	531	536	553	rBV	3871736	4114066	75.78%	12.758%
2	6.451	703	708	721	rBV	4112698	4074718	75.05%	12.636%
3	6.793	762	766	774	rBV	1090290	924466	17.03%	2.867%
4	7.363	858	863	866	rBV	2760909	2658971	48.98%	8.246%
5	8.075	979	984	987	rBV	1369145	1245915	22.95%	3.864%
6	9.151	1161	1167	1170	rBV	5215297	5039775	92.83%	15.629%
7	9.828	1277	1282	1286	rBV	1601551	1407263	25.92%	4.364%
8	10.628	1413	1418	1421	rBV	3557140	3091269	56.94%	9.586%
9	11.322	1532	1536	1539	rBV	1711225	1410672	25.98%	4.375%
10	12.910	1801	1806	1809	rBV	5479061	5429137	100.00%	16.836%
11	13.969	1982	1986	1990	rBV	1578806	1333337	24.56%	4.135%
12	15.039	2164	2168	2173	rVB	50466	59314	1.09%	0.184%
13	15.433	2226	2235	2244	rBV	1006315	1324352	24.39%	4.107%
14	15.827	2298	2302	2307	rVB	45493	64982	1.20%	0.202%
15	16.315	2381	2385	2393	rVB2	38561	68557	1.26%	0.213%




Sum of corrected areas: 32246794

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129869.D
Acq On : 18 Aug 2022 11:22
Operator : CG\JU
Sample : PB146986BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146986BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

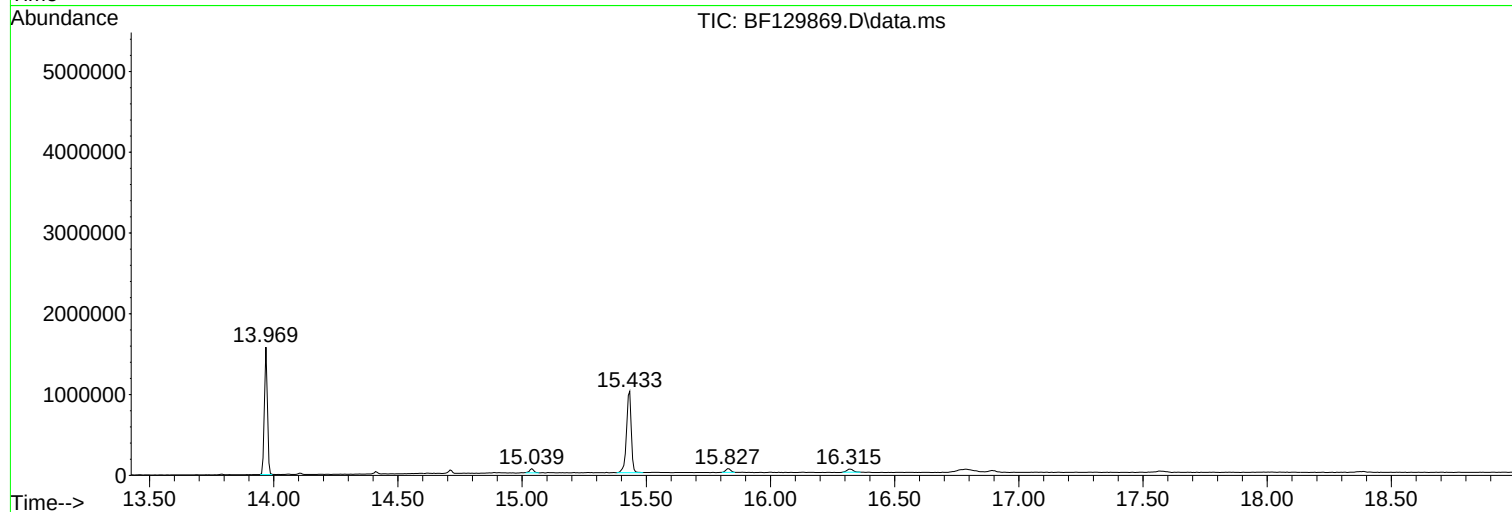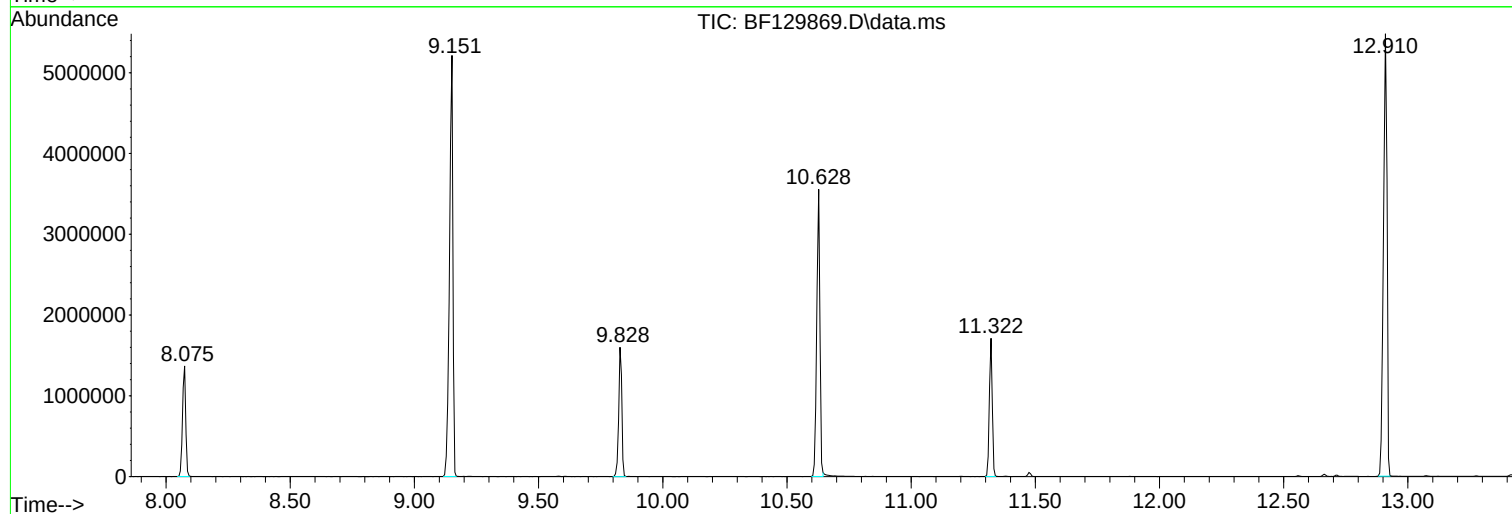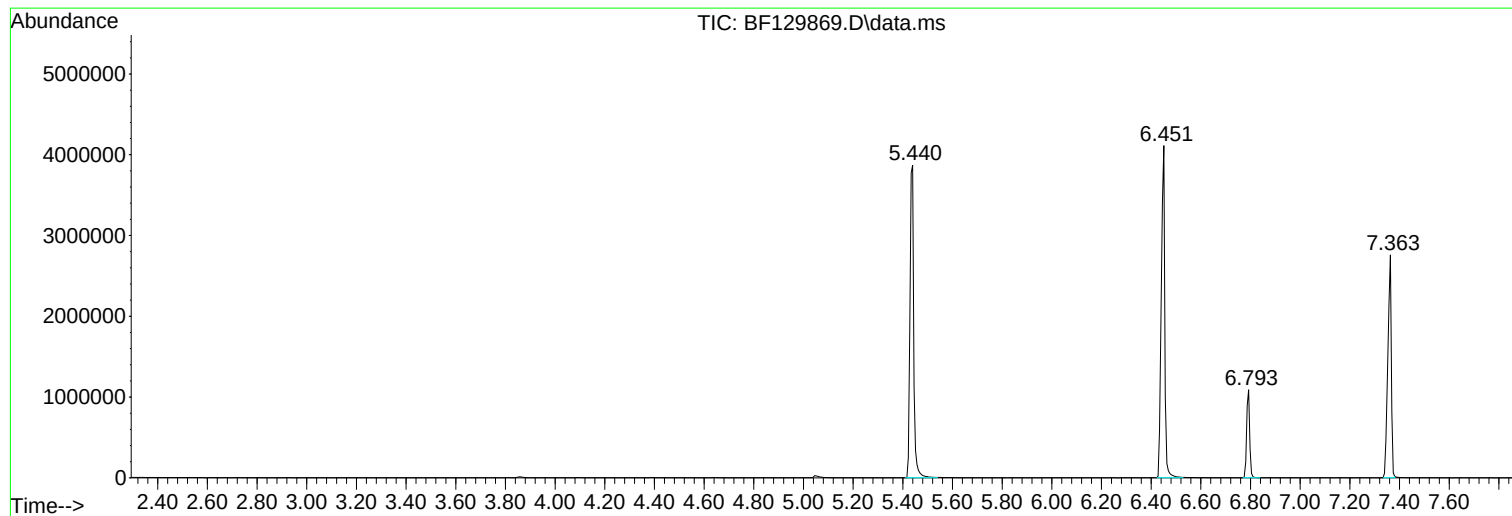

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129869.D
Acq On : 18 Aug 2022 11:22
Operator : CG\JU
Sample : PB146986BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146986BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129869.D
Acq On : 18 Aug 2022 11:22
Operator : CG\JU
Sample : PB146986BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146986BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------