


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
 Data File : BF129867.D
 Acq On : 18 Aug 2022 10:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 18 12:03:10 2022

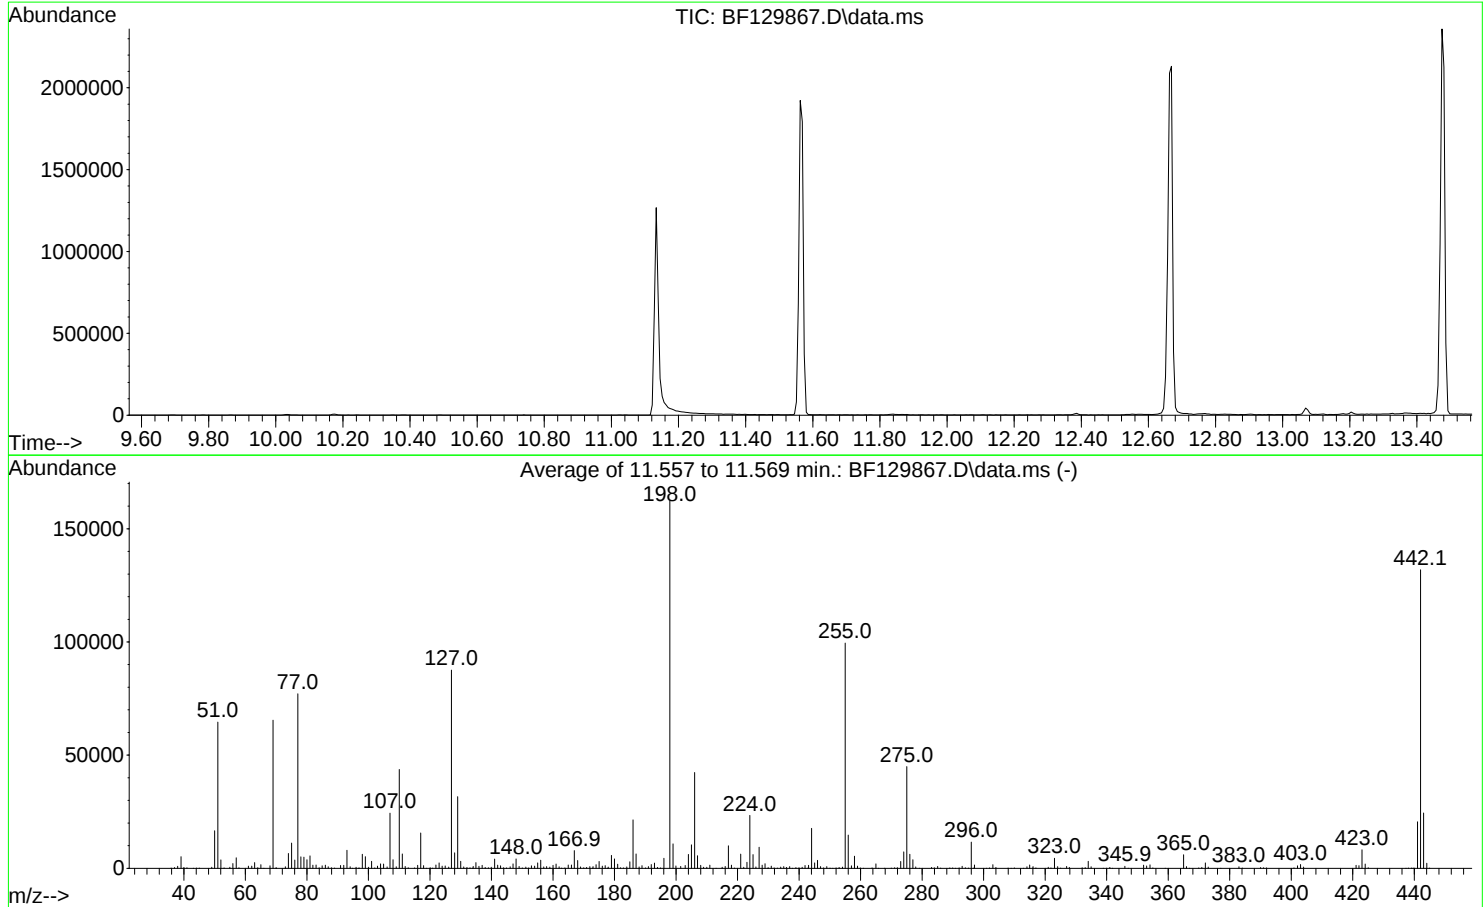




AutoFind: Scans 1576, 1577, 1578; Background Corrected with Scan 1571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	64613	PASS
68	69	0.00	2	1.7	1107	PASS
69	198	0.00	100	40.2	65403	PASS
70	69	0.00	2	0.3	207	PASS
127	198	10	80	53.9	87536	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162533	PASS
199	198	5	9	6.6	10786	PASS
275	198	10	60	27.6	44925	PASS
365	198	1	100	3.7	5948	PASS
441	198	0.01	100	12.6	20517	PASS
442	442	50	100	100.0	131864	PASS
443	442	15	24	18.5	24399	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
 Data File : BF129867.D
 Acq On : 18 Aug 2022 10:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 19 07:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 18 12:03:10 2022
 Response via : Initial Calibration

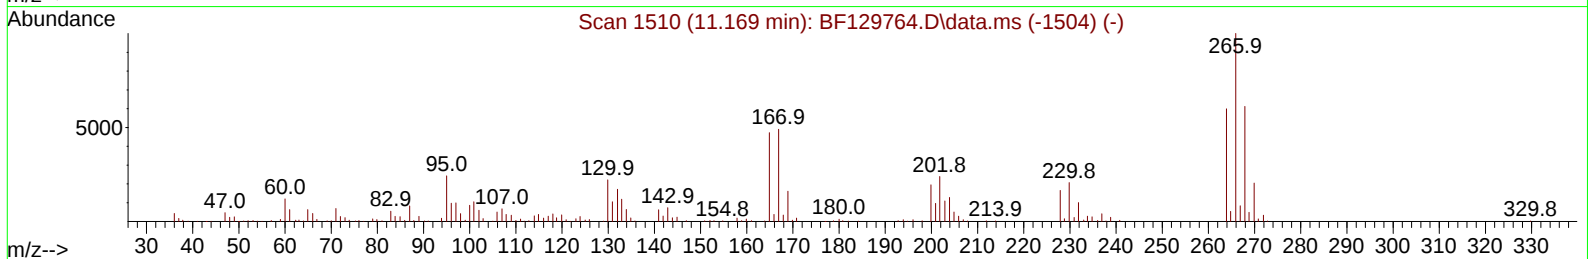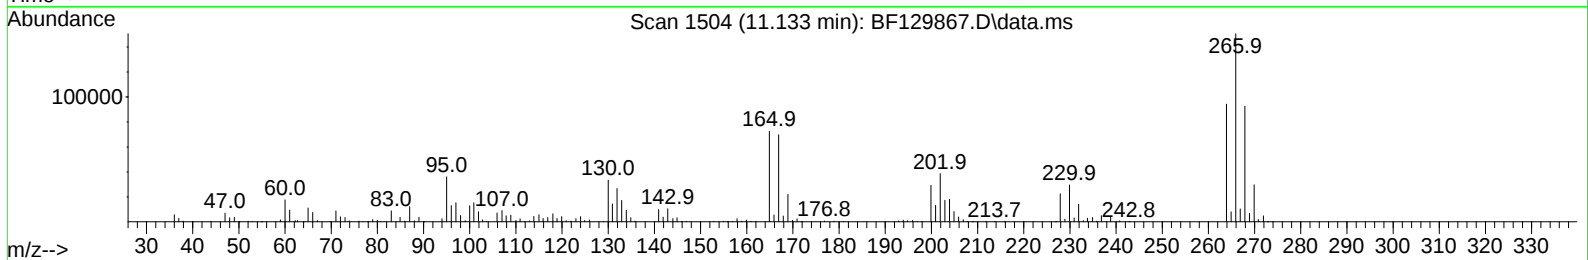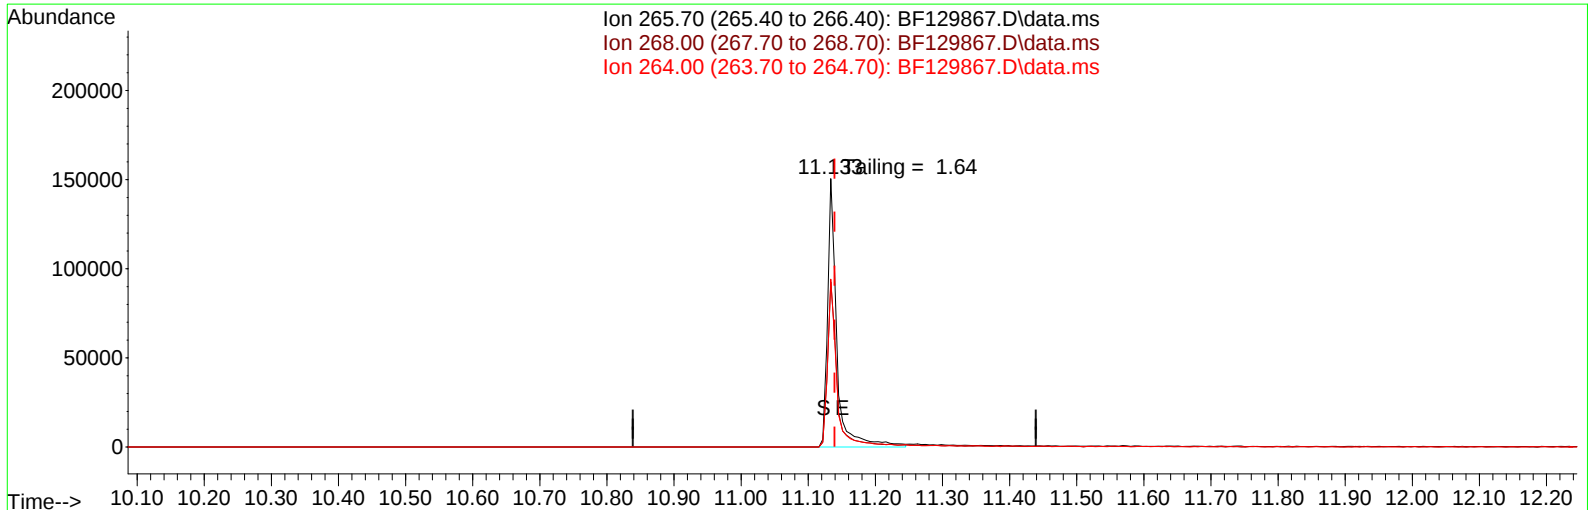

TIC: BF129867.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 83969.20 ng




response 145453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.47
264.00	59.90	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129867.D
Acq On : 18 Aug 2022 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 07:15:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration

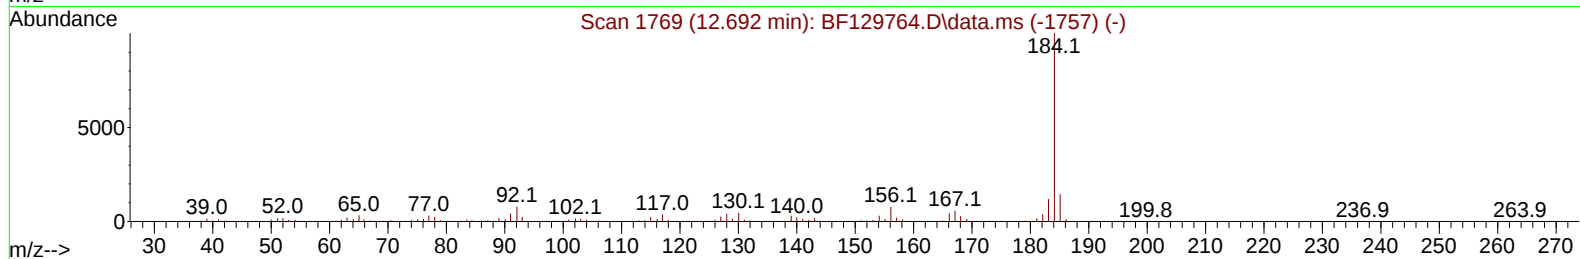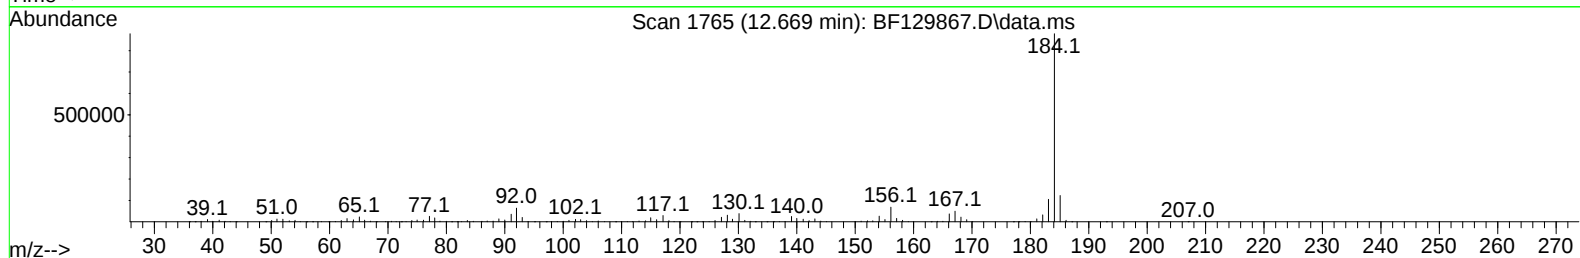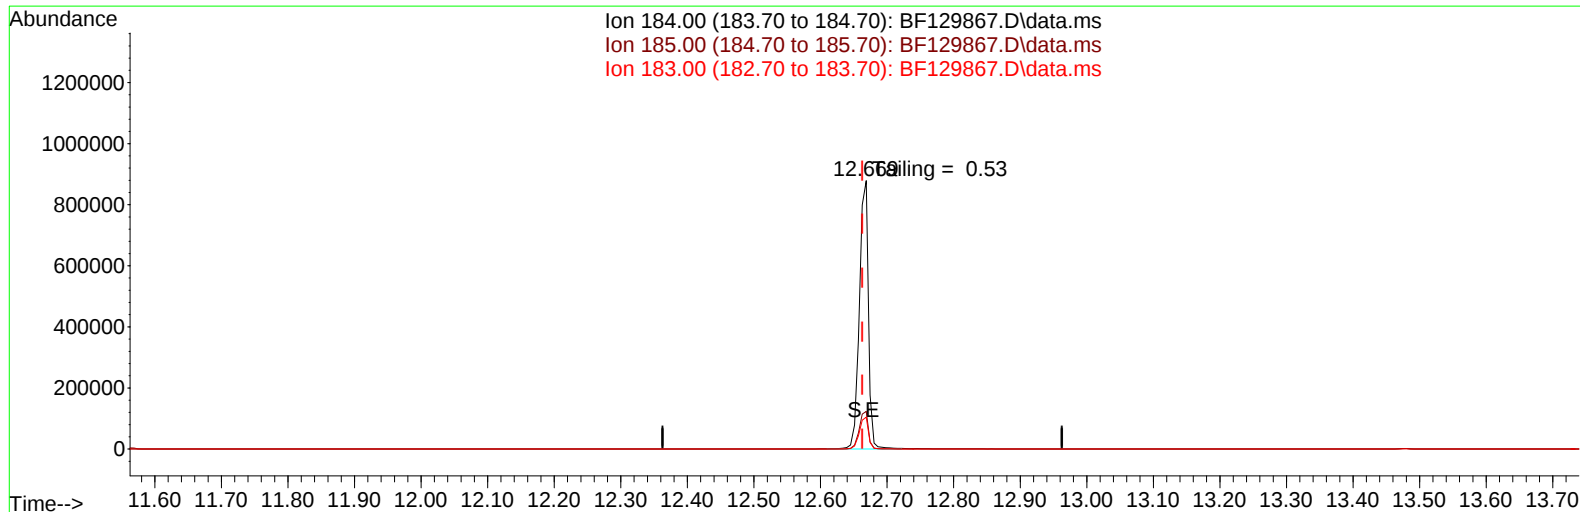

TIC: BF129867.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 150382.43 ng

response 836332

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.01
183.00	11.80	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/18/2022	BNA_F	<u>BF129867.D</u>
Compound Name	Response	Retention Time
DDT	416813	13.474
DDD	3786	13.204
DDE	380	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4166	420979	0.99

Instrument :
BNA_F
ClientSampleId :
DFTPP