


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
 Data File : BF129878.D
 Acq On : 18 Aug 2022 16:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 18 12:03:10 2022

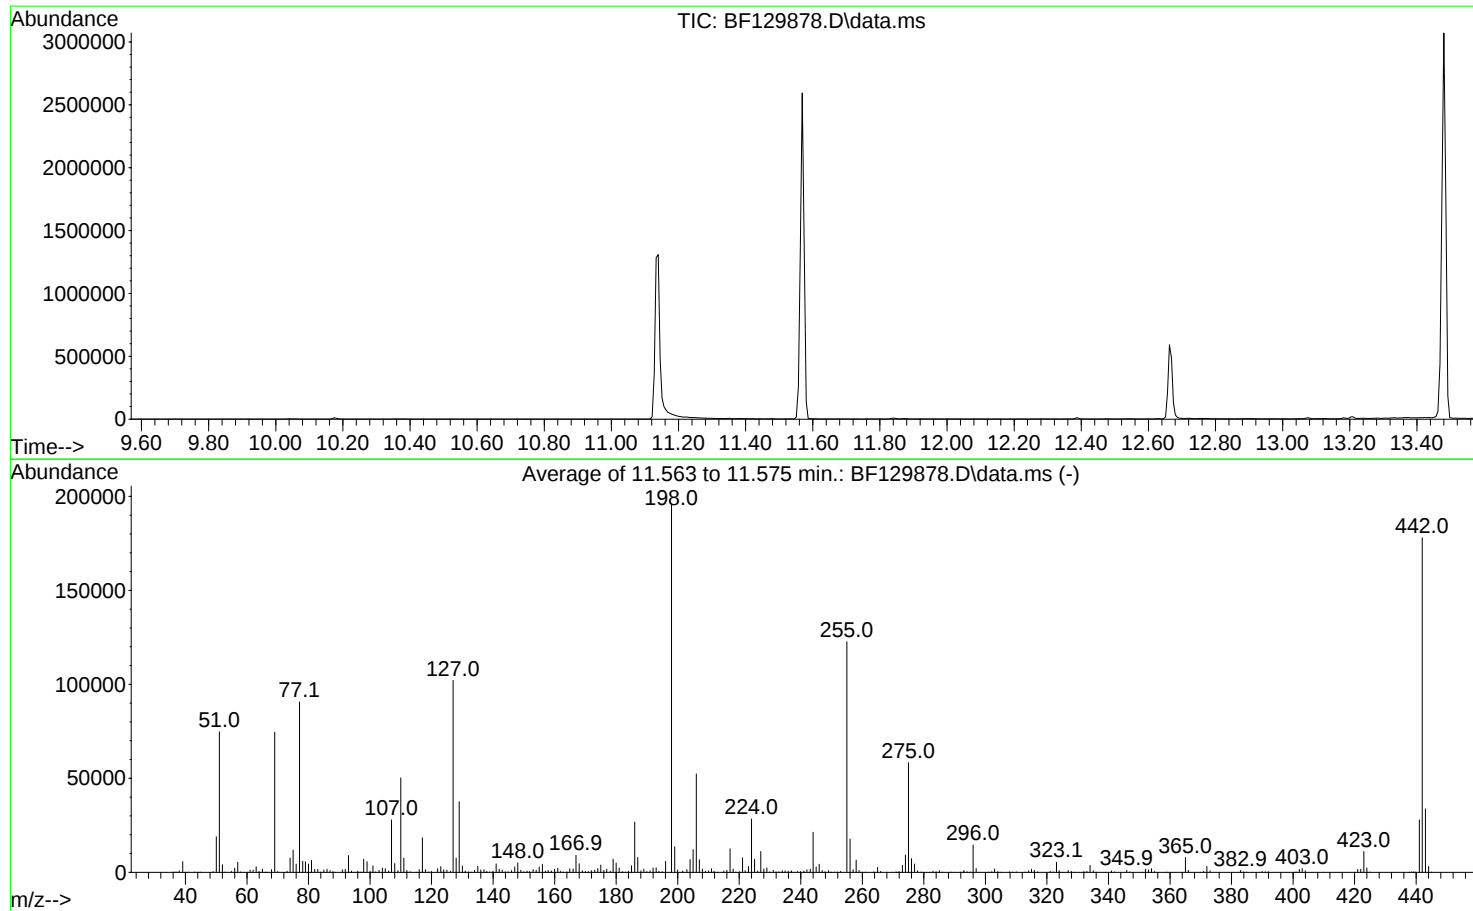




AutoFind: Scans 1577, 1578, 1579; Background Corrected with Scan 1572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	74760	PASS
68	69	0.00	2	1.8	1375	PASS
69	198	0.00	100	38.1	74571	PASS
70	69	0.00	2	0.5	373	PASS
127	198	10	80	52.2	102107	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	195733	PASS
199	198	5	9	6.9	13585	PASS
275	198	10	60	29.8	58347	PASS
365	198	1	100	4.0	7880	PASS
441	198	0.01	100	14.2	27850	PASS
442	442	50	100	100.0	178019	PASS
443	442	15	24	18.9	33724	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\  
Data File : BF129878.D  
Acq On    : 18 Aug 2022  16:24  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 05:02:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration

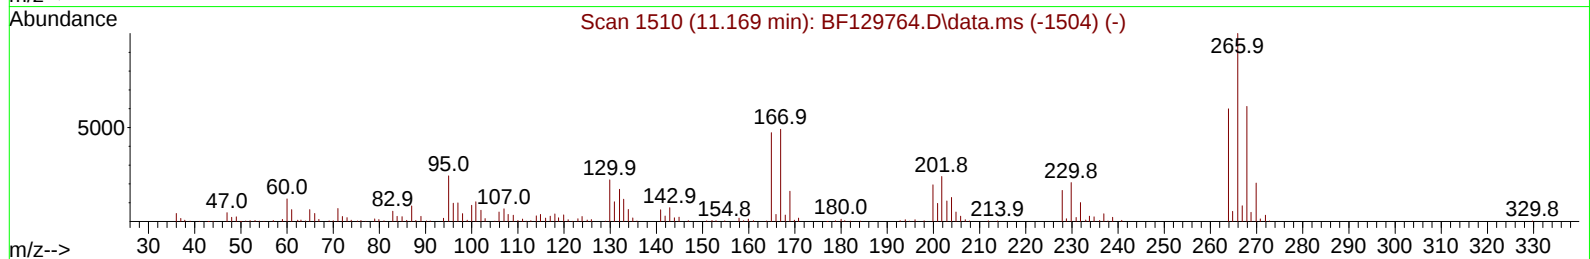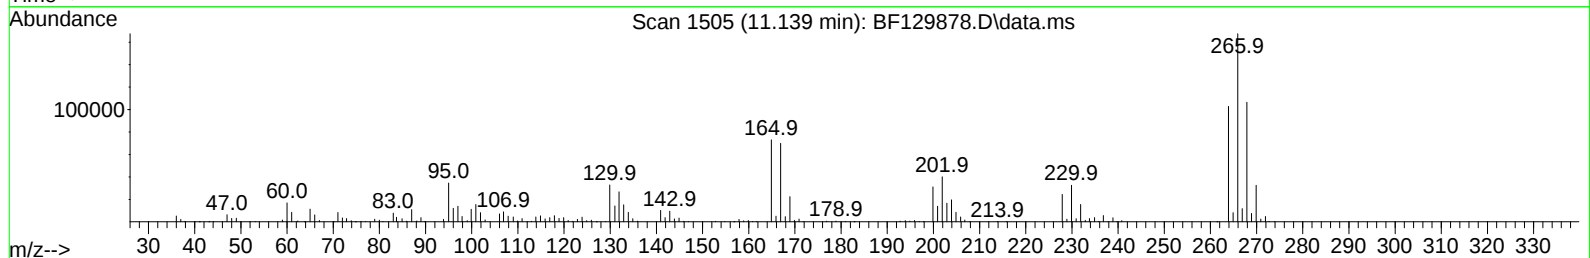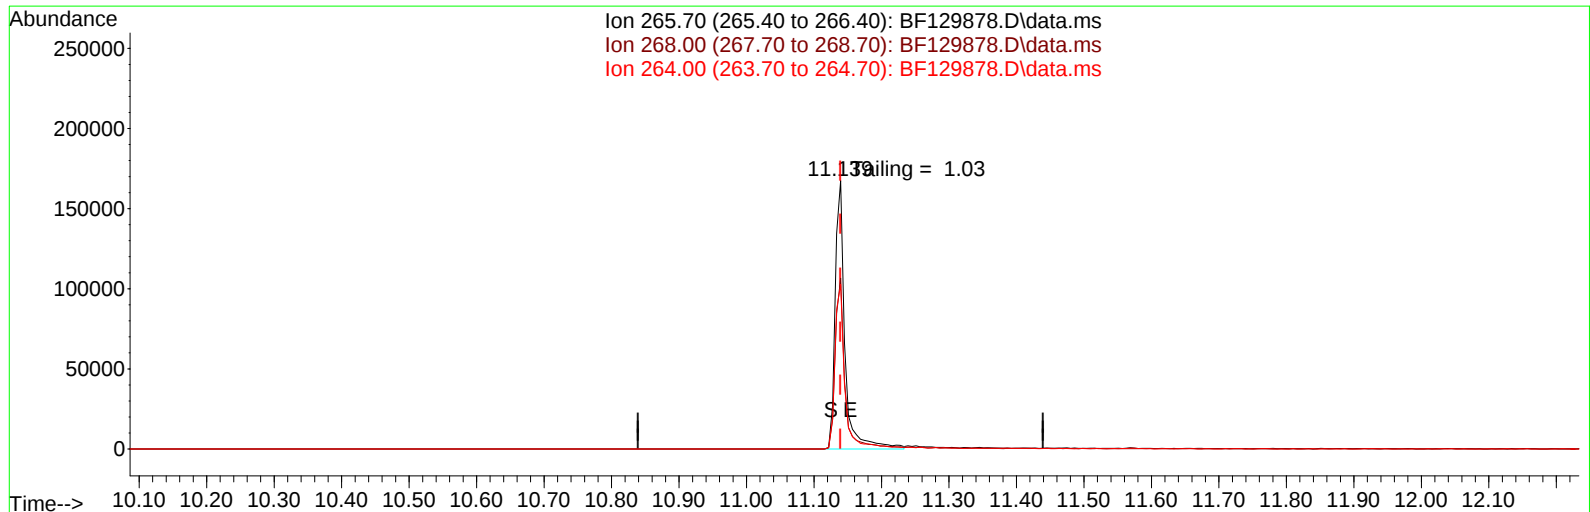

TIC: BF129878.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 496402.47 ng




response **169562**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.61
264.00	59.90	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081822\
Data File : BF129878.D
Acq On : 18 Aug 2022 16:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 19 05:02:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 18 12:03:10 2022
Response via : Initial Calibration

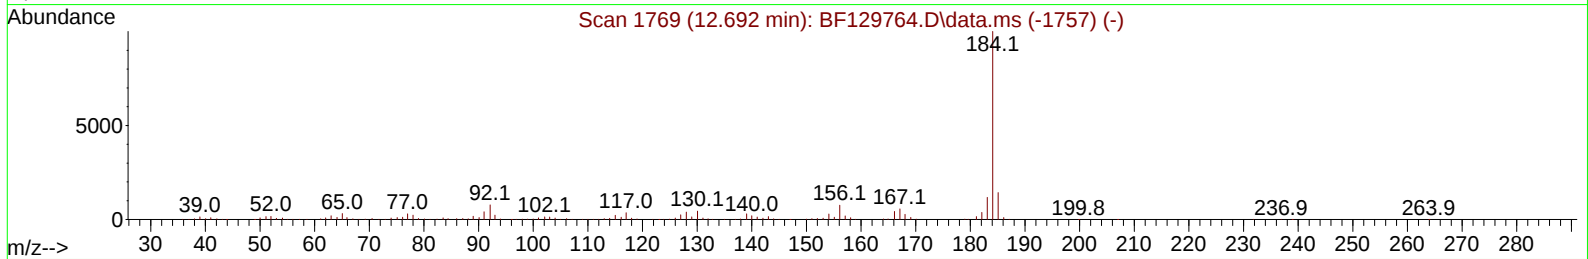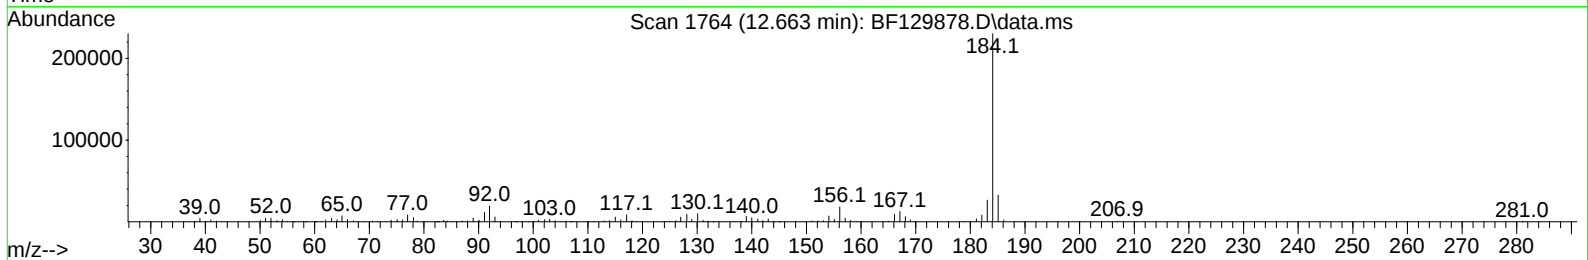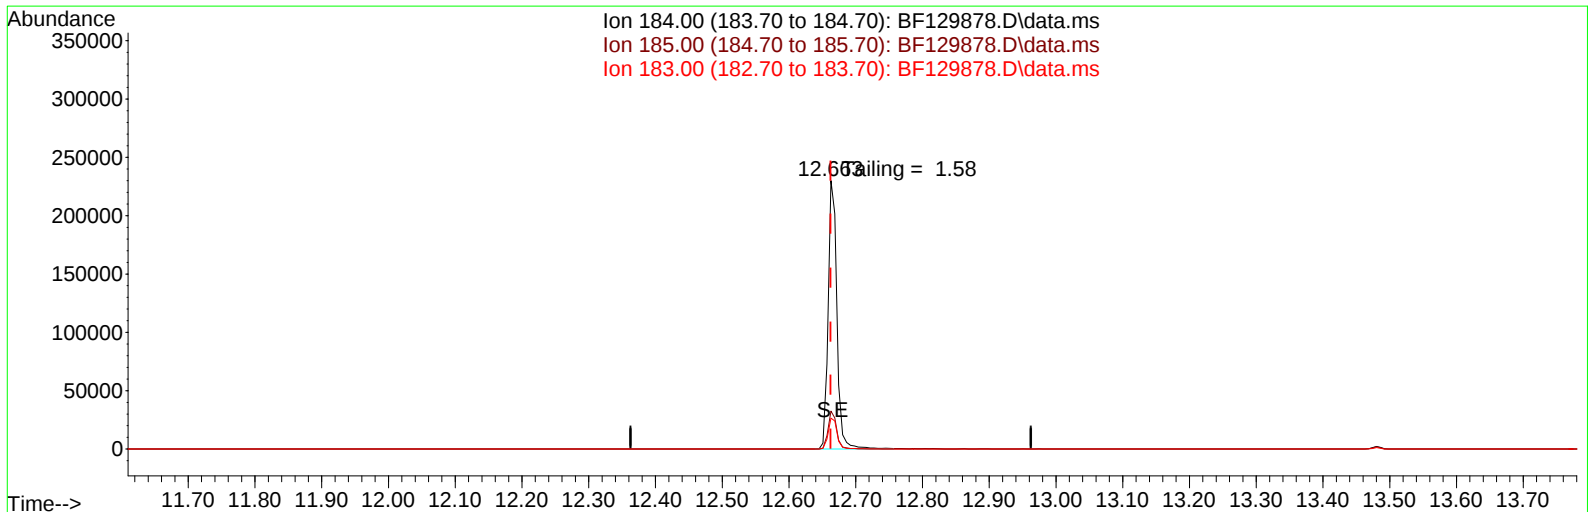

TIC: BF129878.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 65799.48 ng

response 211502

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.16
183.00	11.80	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/18/2022	BNA_F	<u>BF129878.D</u>
Compound Name	Response	Retention Time
DDT	488268	13.48
DDD	4424	13.21
DDE	333	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4757	493025	0.96

Instrument :
BNA_F
ClientSampleId :
DFTPP