

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081825\
Data File : BF143433.D
Acq On : 18 Aug 2025 11:02
Operator : RC/JU
Sample : PB169256BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169256BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.322	9	22	31	rVB	32164	60930	1.39%	0.259%
2	5.569	568	574	596	rBV	1904953	2554798	58.20%	10.849%
3	6.557	736	742	775	rBV	1815189	2557384	58.26%	10.860%
4	6.928	799	805	810	rBV	590400	751011	17.11%	3.189%
5	7.481	893	899	916	rBV	1734243	2472665	56.33%	10.500%
6	8.204	1016	1022	1043	rBV	742734	1005796	22.91%	4.271%
7	9.281	1198	1205	1210	rBV	3306631	4389720	100.00%	18.642%
8	9.963	1315	1321	1334	rBV	872468	1157661	26.37%	4.916%
9	10.745	1449	1454	1484	rBV	1279392	1831030	41.71%	7.776%
10	11.445	1568	1573	1591	rBV	909970	1182080	26.93%	5.020%
11	13.027	1836	1842	1862	rBV	3181094	4287752	97.68%	18.208%
12	14.086	2016	2022	2041	rBV	494144	708955	16.15%	3.011%
13	15.574	2269	2275	2294	rBV	342031	588303	13.40%	2.498%




Sum of corrected areas: 23548085

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081825\
Data File : BF143433.D
Acq On : 18 Aug 2025 11:02
Operator : RC/JU
Sample : PB169256BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169256BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

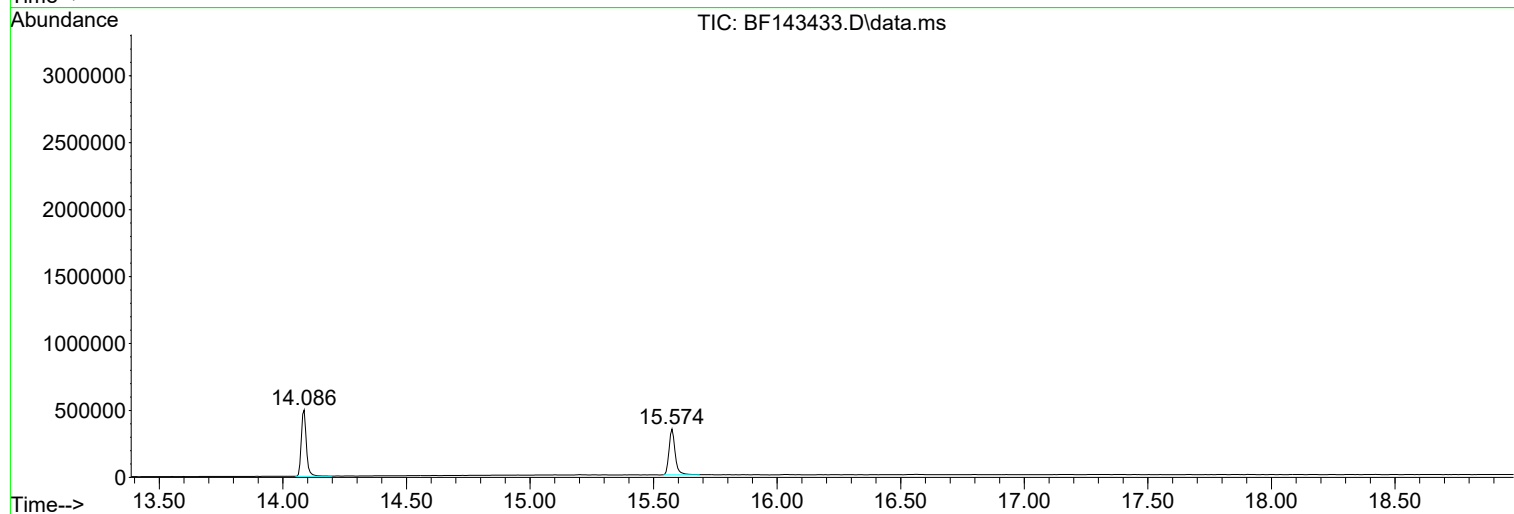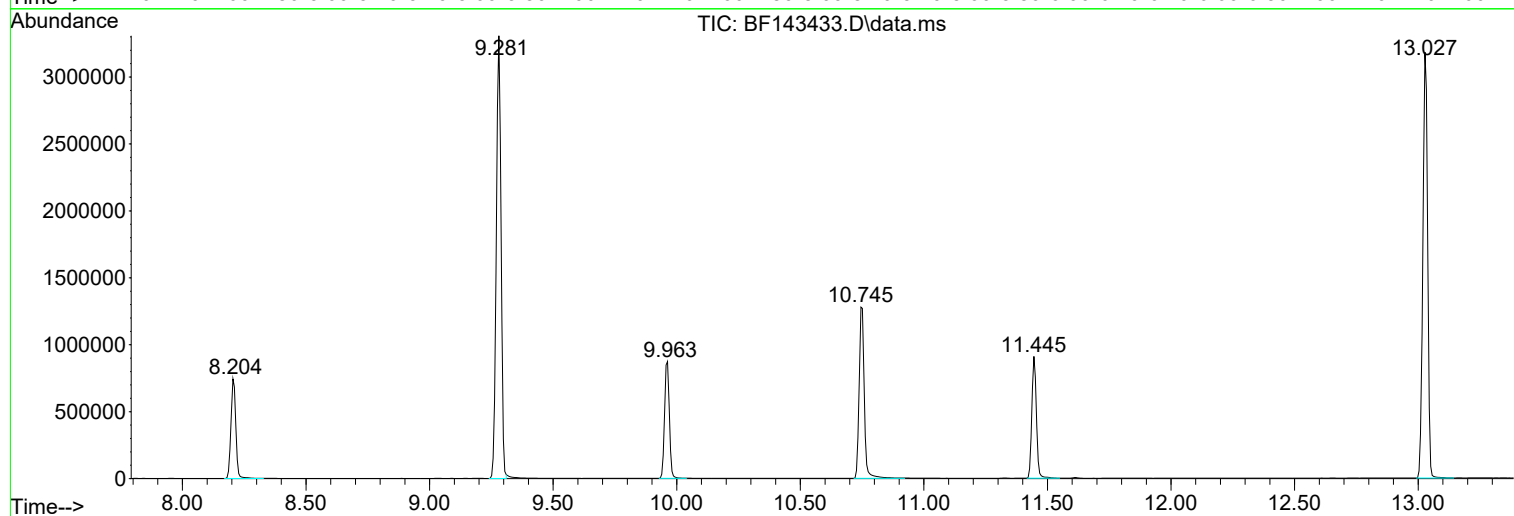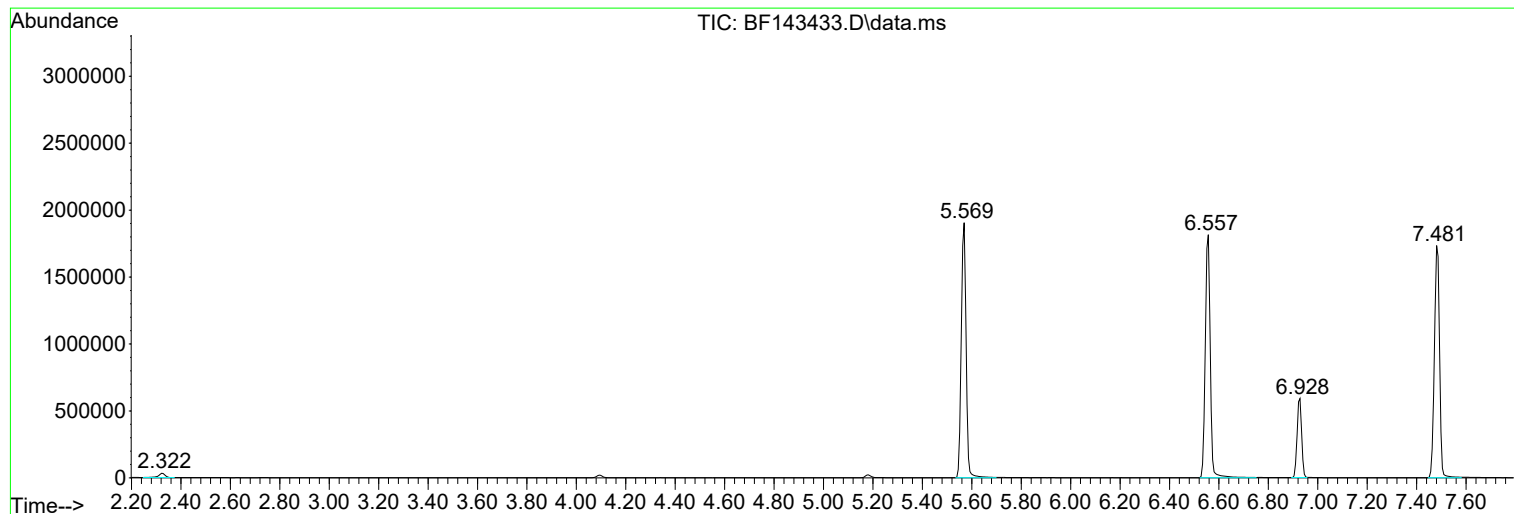

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081825\
Data File : BF143433.D
Acq On : 18 Aug 2025 11:02
Operator : RC/JU
Sample : PB169256BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169256BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081825\
Data File : BF143433.D
Acq On : 18 Aug 2025 11:02
Operator : RC/JU
Sample : PB169256BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169256BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------