

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081915\
 Data File : BF081108.D
 Acq On : 20 Aug 2015 5:11
 Operator : UM/IZ
 Sample : G3304-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2PM-MLSP-10

Quant Time: Aug 20 06:51:54 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 17 17:57:25 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	61629	20.00	ng	-0.04
21) Naphthalene-d8	7.88	136	232398	20.00	ng	-0.03
38) Acenaphthene-d10	9.61	164	104793	20.00	ng	-0.04
63) Phenanthrene-d10	11.09	188	232343	20.00	ng	-0.04
75) Chrysene-d12	13.71	240	205937	20.00	ng	-0.04
86) Perylene-d12	15.04	264	158927	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.17	112	506957	123.73	ng	-0.02
7) Phenol-d6	6.24	99	741752	138.75	ng	-0.02
23) Nitrobenzene-d5	7.16	82	432645	85.04	ng	-0.03
41) 2,4,6-Tribromophenol	10.40	330	131723	145.01	ng	-0.04
44) 2-Fluorobiphenyl	8.95	172	710137	88.79	ng	-0.04
78) Terphenyl-d14	12.68	244	765274	79.67	ng	-0.03


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081915\
Data File : BF081108.D
Acq On : 20 Aug 2015 5:11
Operator : UM/IZ
Sample : G3304-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2PM-MLSP-10

Quant Time: Aug 20 06:51:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 17 17:57:25 2015
Response via : Initial Calibration

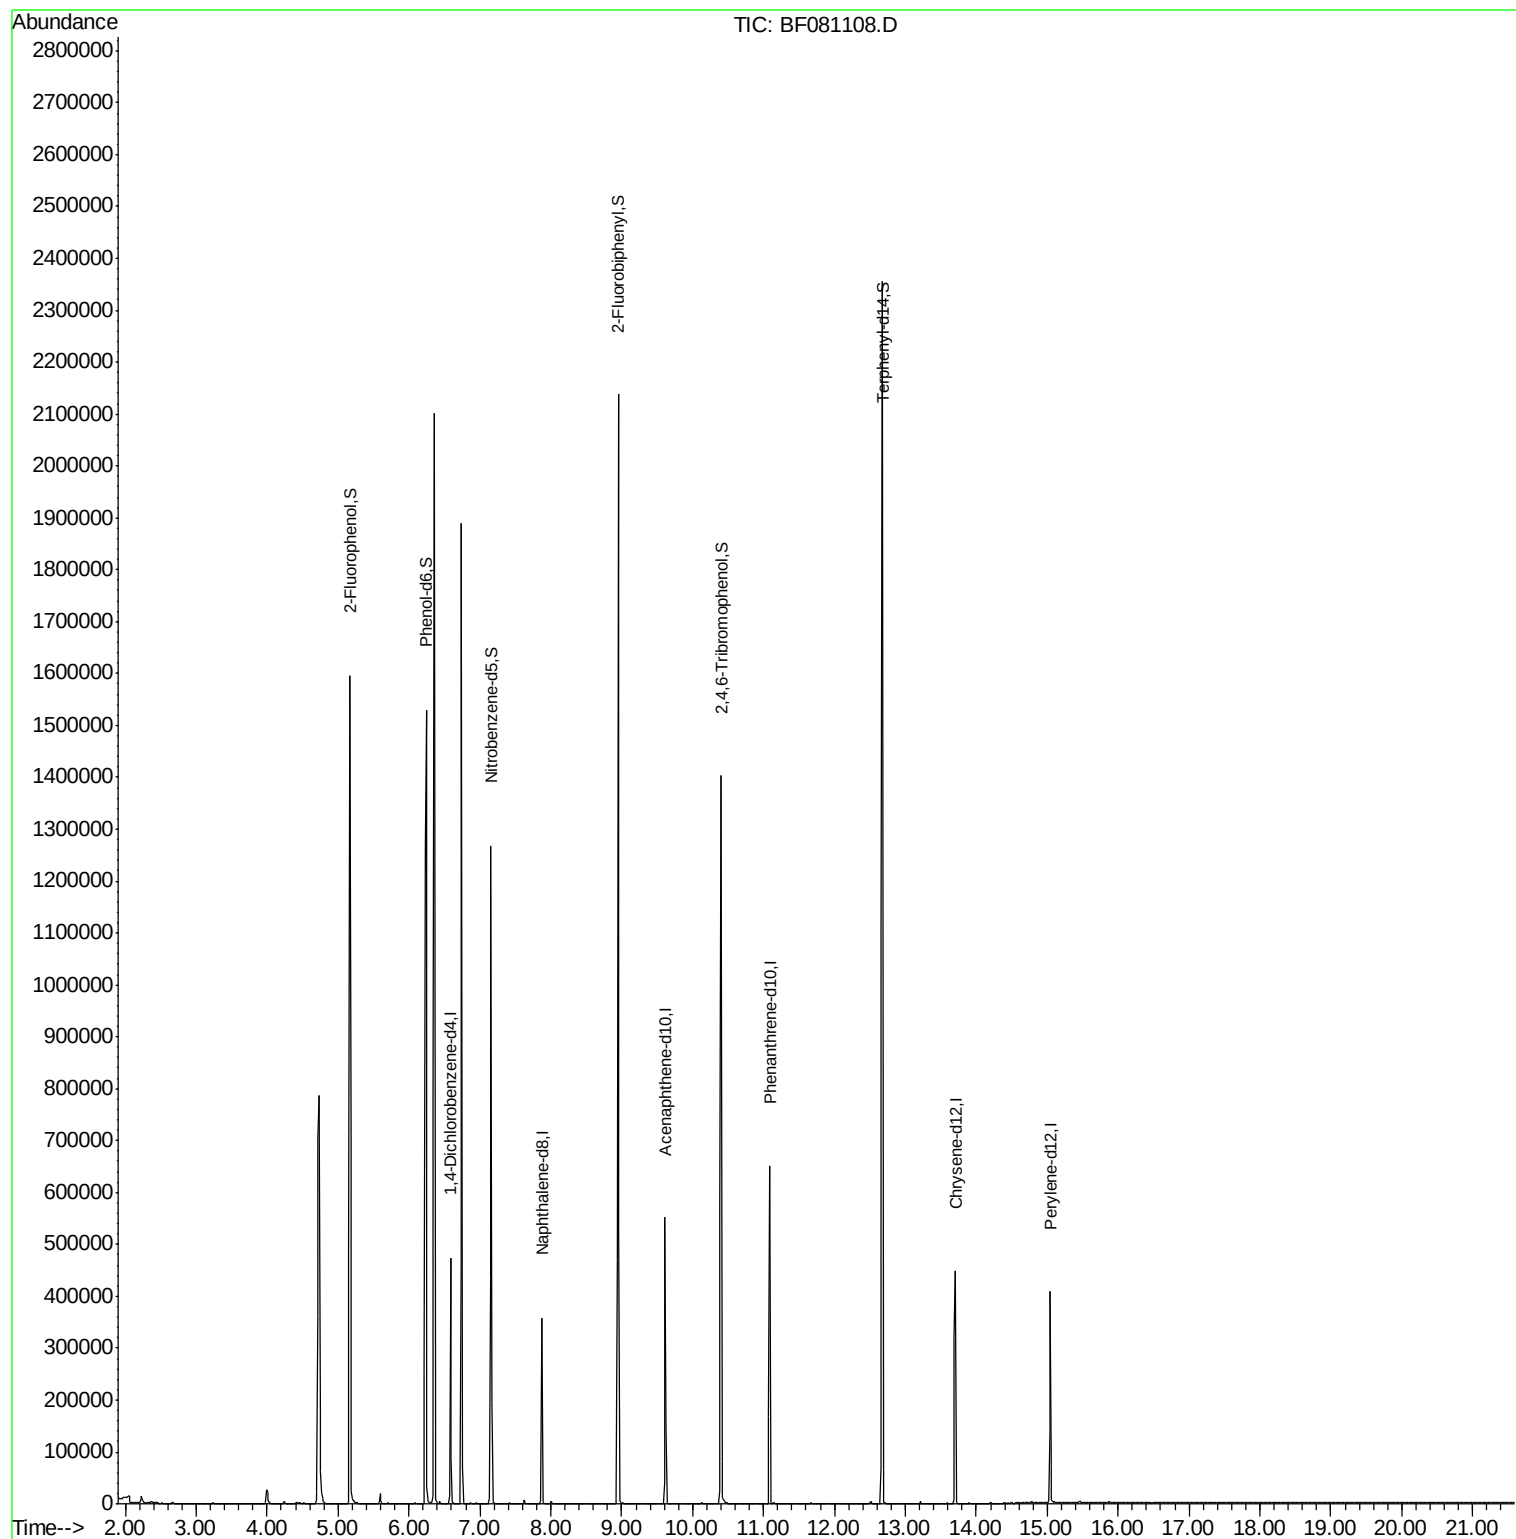

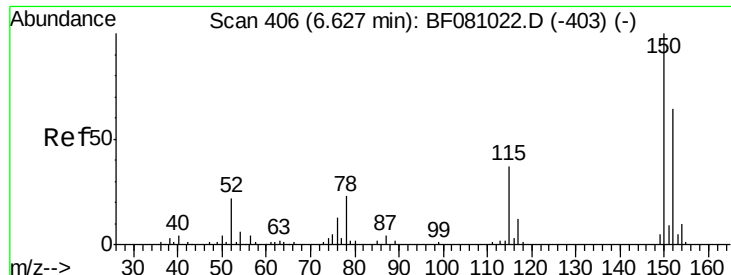

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 411

Delta R.T. -0.04 min

Lab File: BF081108.D

Acq: 20 Aug 2015 5:11

Instrument :

BNA_F

ClientSampleId :

E2PM-MLSP-10


Tgt Ion:152 Resp: 61629

Ion Ratio Lower Upper

152 100

150 160.0 123.8 185.6




115 70.5 52.1 78.1

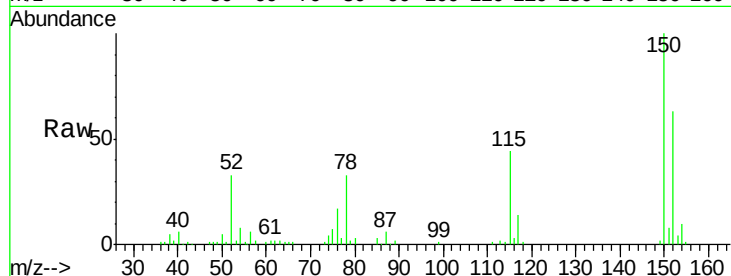

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

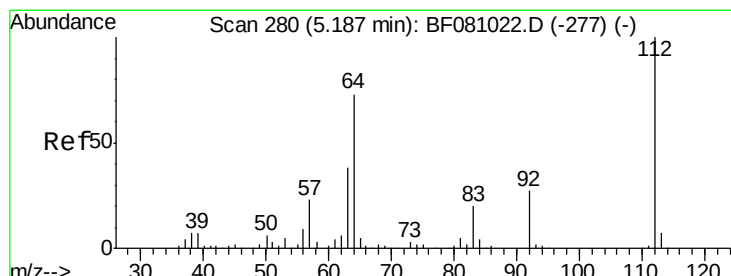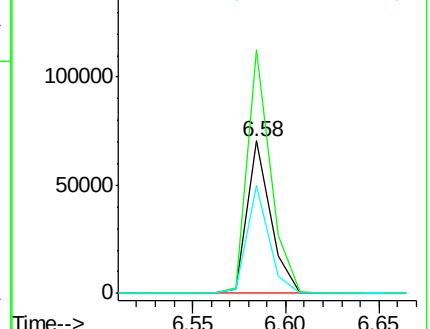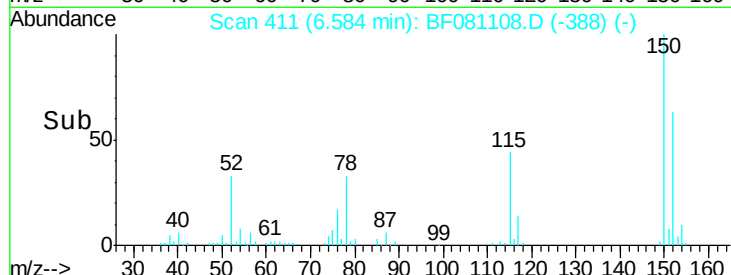

#5

2-Fluorophenol

Concen: 123.73 ng

RT: 5.17 min Scan# 287

Delta R.T. -0.02 min

Lab File: BF081108.D

Acq: 20 Aug 2015 5:11


Tgt Ion:112 Resp: 506957

Ion Ratio Lower Upper

112 100

64 79.6 66.9 100.3



63 41.6 38.1 57.1

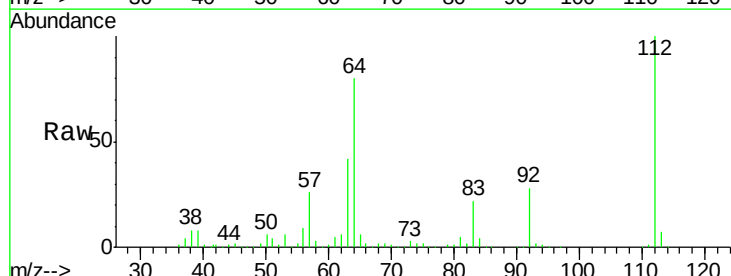


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

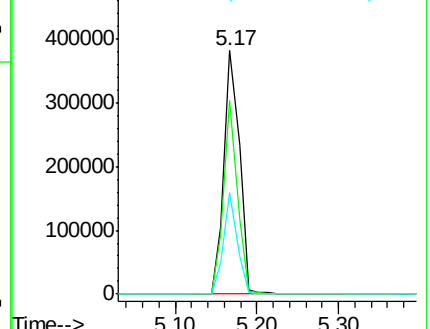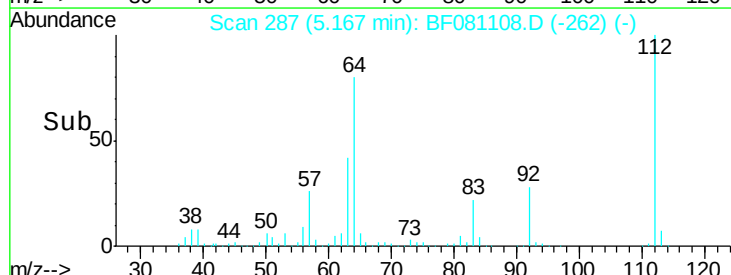

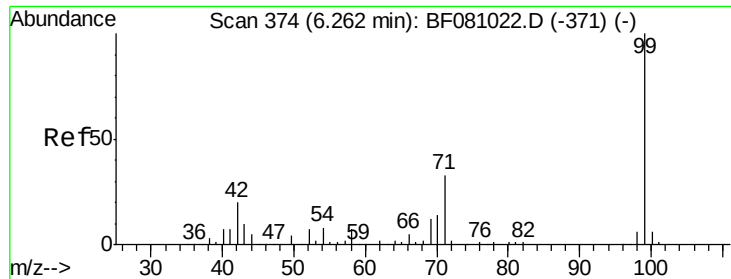

#7

Phenol-d6

Concen: 138.75 ng

RT: 6.24 min Scan# 381

Delta R.T. -0.02 min

Lab File: BF081108.D

Acq: 20 Aug 2015 5:11

Instrument :

BNA_F

ClientSampleId :

E2PM-MLSP-10


Tgt Ion: 99 Resp: 741752

Ion Ratio Lower Upper

99 100

42 16.9 19.6 29.4#




71 31.9 31.2 46.8

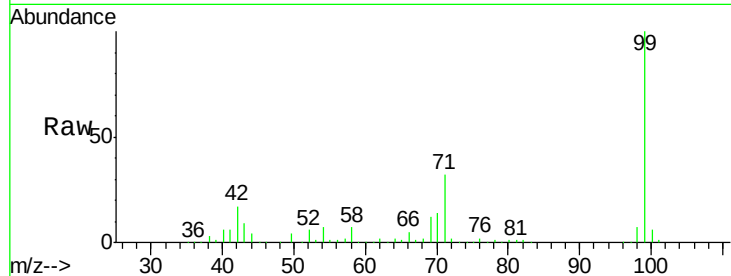

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

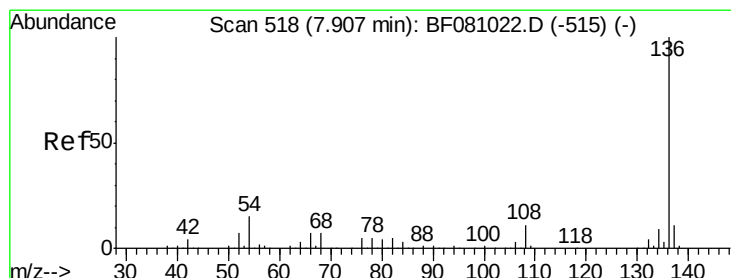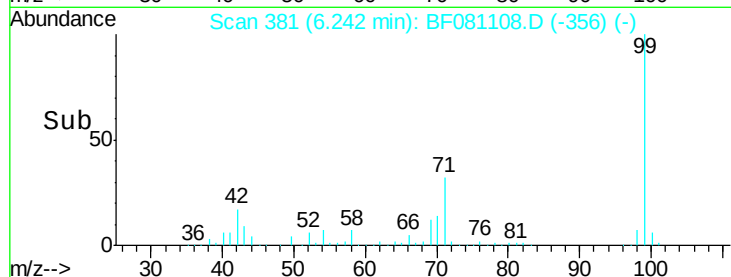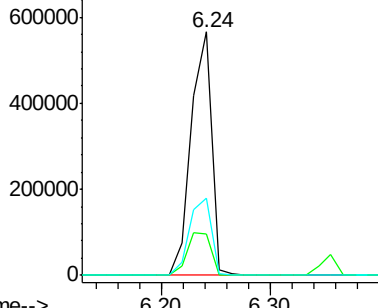

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.88 min Scan# 524

Delta R.T. -0.03 min

Lab File: BF081108.D

Acq: 20 Aug 2015 5:11

Tgt Ion: 136 Resp: 232398


Ion Ratio Lower Upper

136 100

137 10.8 8.2 12.2

54 8.1 7.7 11.5

68 4.5 3.4 5.2


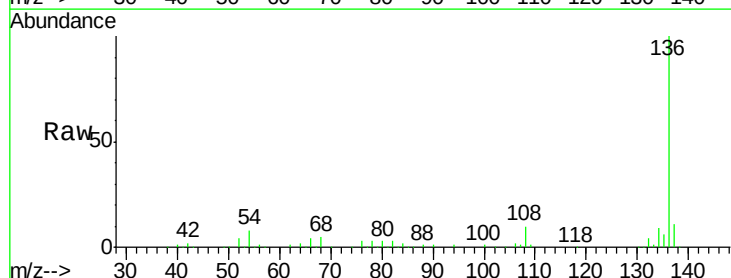



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



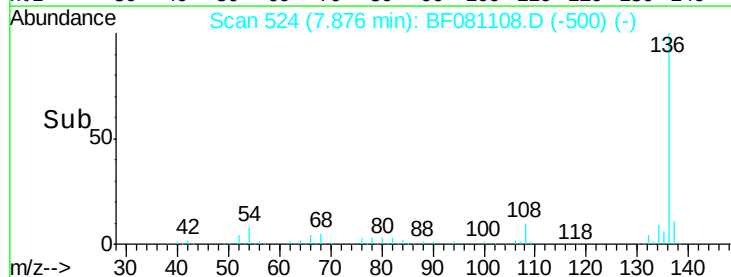
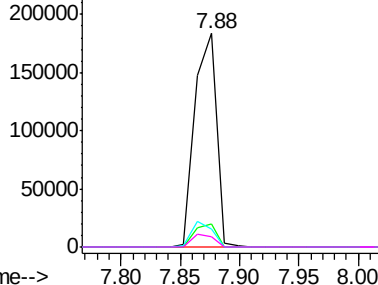


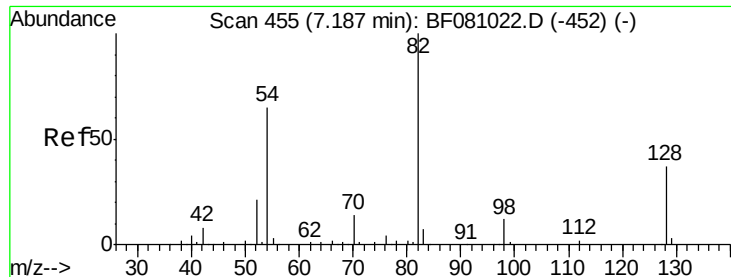

#23
 Nitrobenzene-d5
 Concen: 85.04 ng
 RT: 7.16 min Scan# 461
 Delta R.T. -0.03 min
 Lab File: BF081108.D
 Acq: 20 Aug 2015 5:11




Instrument :
 BNA_F
 ClientSampleId :
 E2PM-MLSP-10


Tgt Ion: 82 Resp: 432645
 Ion Ratio Lower Upper
 82 100
 128 37.6 28.6 42.8
 54 66.3 55.1 82.7

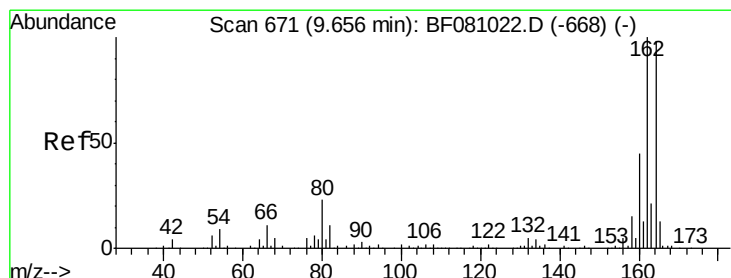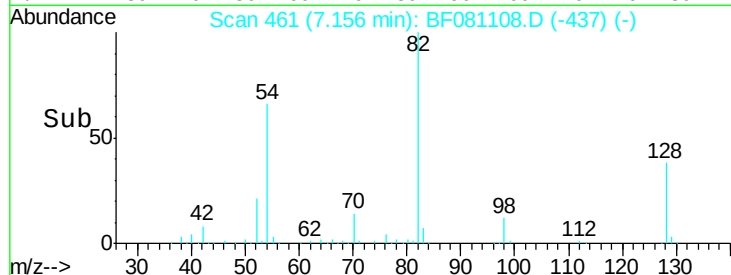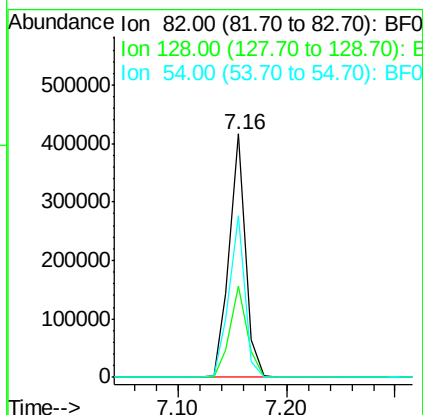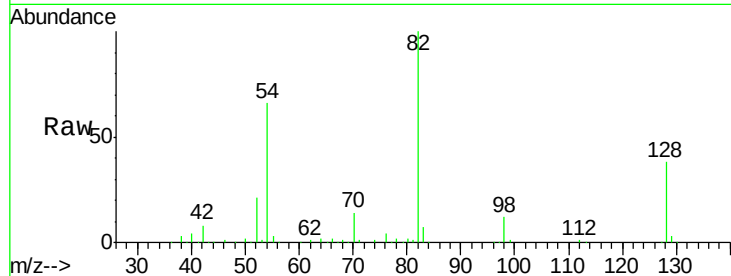

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.61 min Scan# 676
 Delta R.T. -0.04 min
 Lab File: BF081108.D
 Acq: 20 Aug 2015 5:11

Tgt Ion: 164 Resp: 104793
 Ion Ratio Lower Upper
 164 100
 162 103.6 83.8 125.8
 160 46.0 39.8 59.8

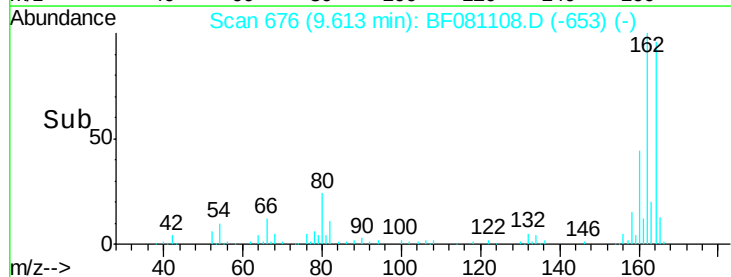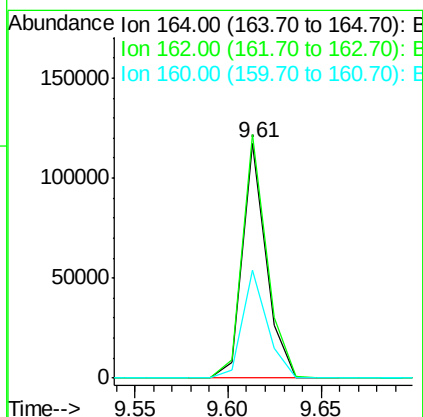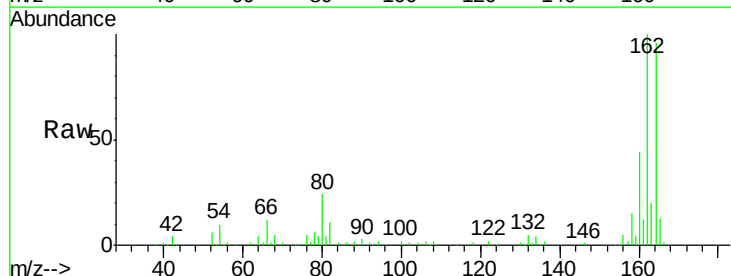


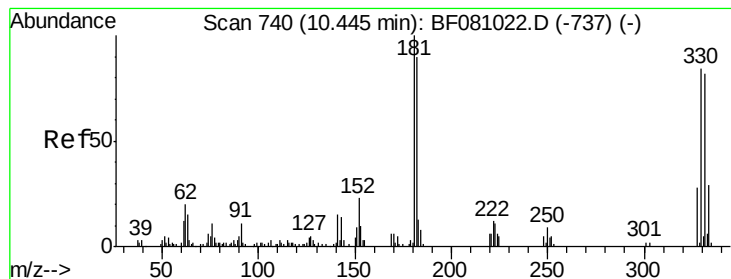




#41
 2,4,6-Tribromophenol
 Concen: 145.01 ng
 RT: 10.40 min Scan# 745
 Delta R.T. -0.04 min
 Lab File: BF081108.D
 Acq: 20 Aug 2015 5:11

Instrument :
 BNA_F
 ClientSampleId :
 E2PM-MLSP-10

Tgt Ion: 330 Resp: 131723
 Ion Ratio Lower Upper
 330 100
 332 94.4 77.3 115.9
 141 55.8 44.9 67.3

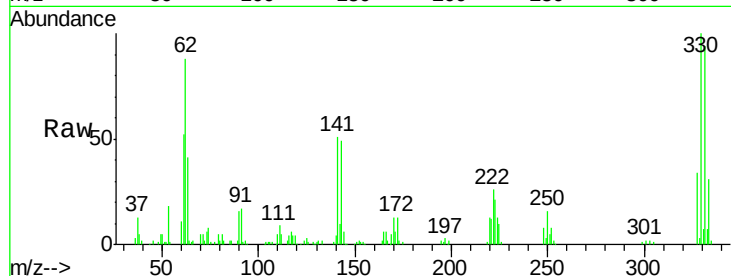


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

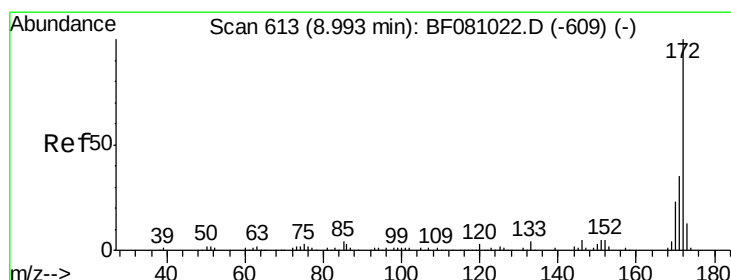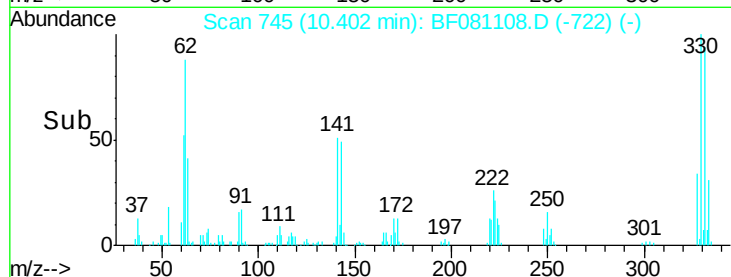
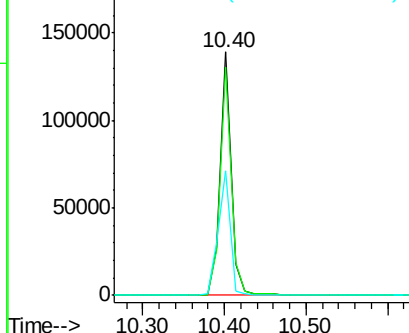



#44
 2-Fluorobiphenyl
 Concen: 88.79 ng
 RT: 8.95 min Scan# 618
 Delta R.T. -0.04 min
 Lab File: BF081108.D
 Acq: 20 Aug 2015 5:11

Tgt Ion: 172 Resp: 710137
 Ion Ratio Lower Upper
 172 100
 171 36.2 28.9 43.3
 170 24.6 19.4 29.2

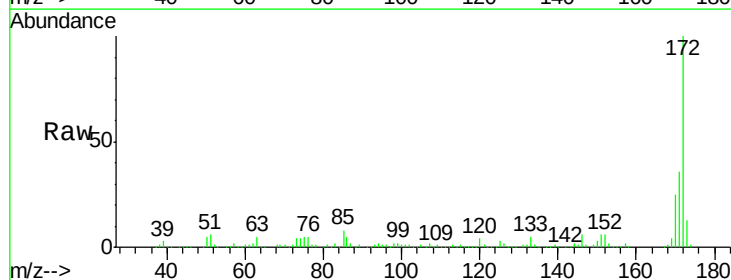

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

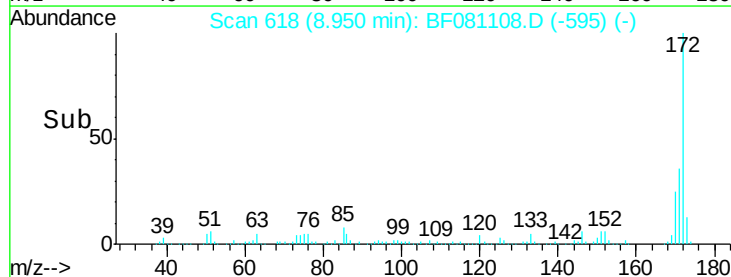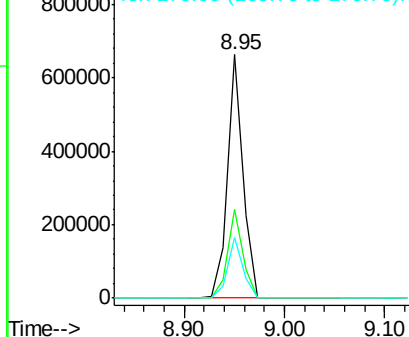


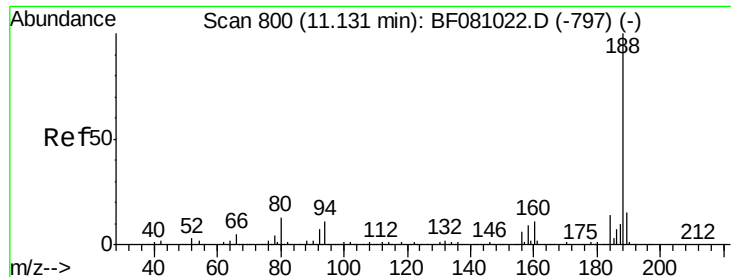




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.09 min Scan# 805
Delta R.T. -0.04 min
Lab File: BF081108.D
Acq: 20 Aug 2015 5:11

Instrument :
BNA_F
ClientSampleId :
E2PM-MLSP-10

Tgt Ion:188 Resp: 232343
Ion Ratio Lower Upper
188 100
94 8.4 8.2 12.2
80 9.1 9.5 14.3#

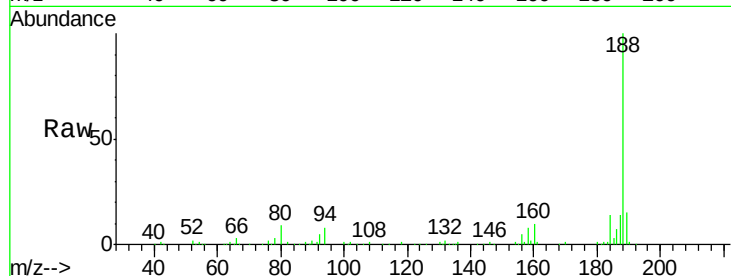


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

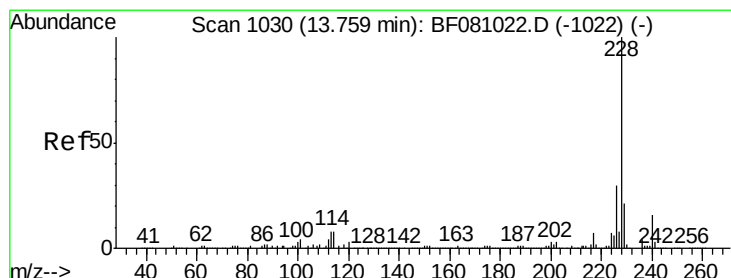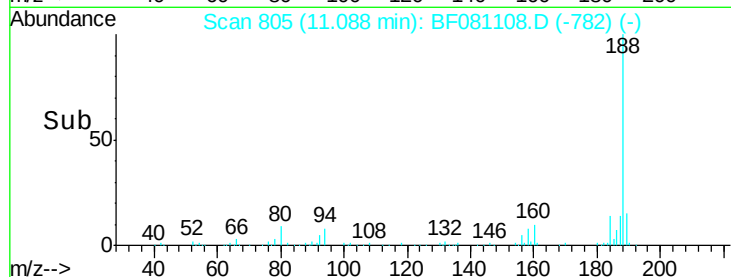
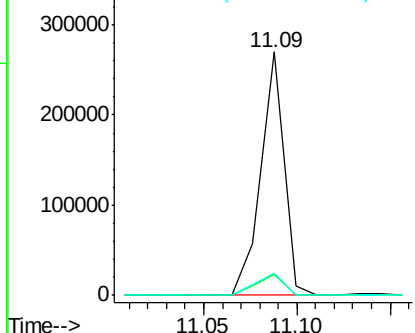



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.71 min Scan# 1034
Delta R.T. -0.04 min
Lab File: BF081108.D
Acq: 20 Aug 2015 5:11

Tgt Ion:240 Resp: 205937
Ion Ratio Lower Upper
240 100
120 8.0 5.6 8.4
236 26.0 20.6 30.8

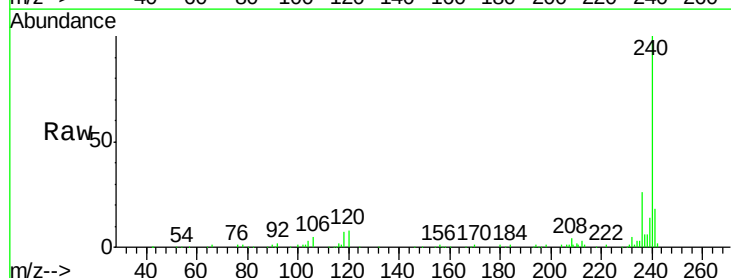

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



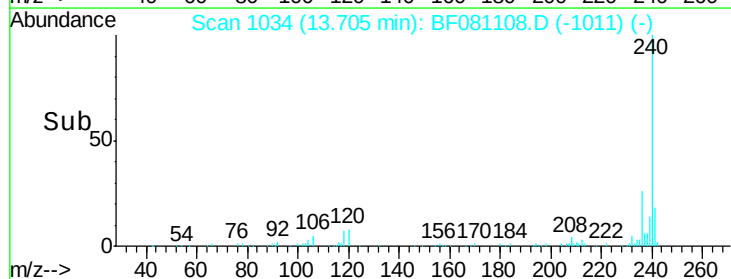
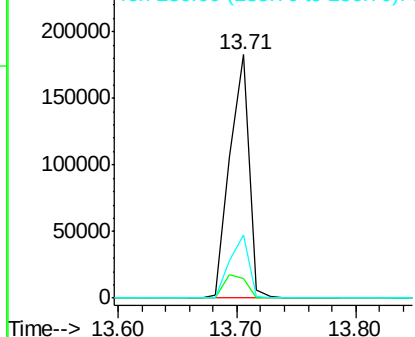


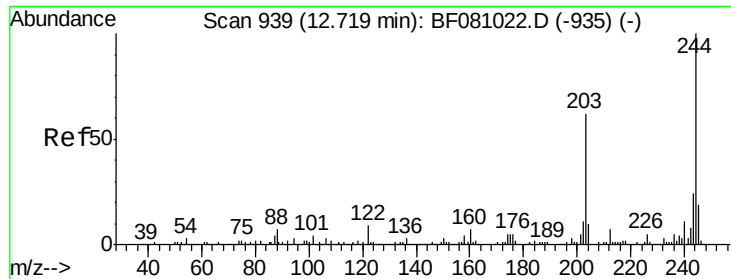

#78
 Terphenyl-d14
 Concen: 79.67 ng
 RT: 12.68 min Scan# 944
 Delta R.T. -0.03 min
 Lab File: BF081108.D
 Acq: 20 Aug 2015 5:11

Instrument :
 BNA_F
 ClientSampleId :
 E2PM-MLSP-10

Tgt Ion: 244 Resp: 765274
 Ion Ratio Lower Upper
 244 100
 212 7.8 5.8 8.8
 122 13.4 8.2 12.4#

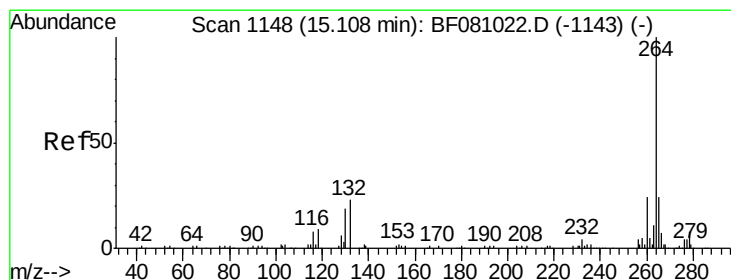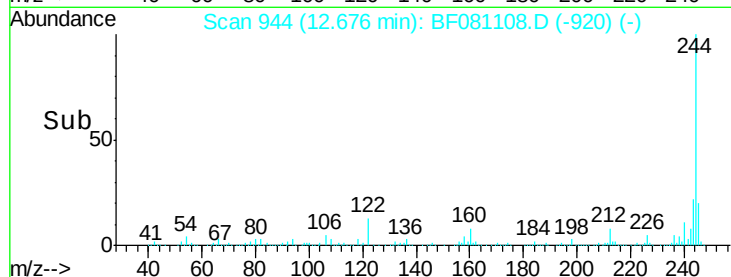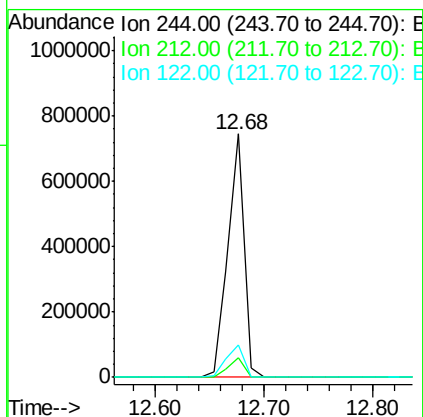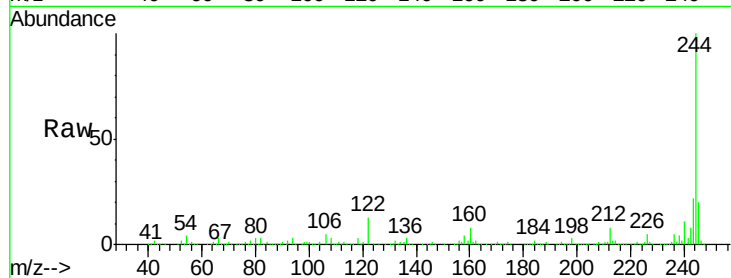

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.04 min Scan# 1151
 Delta R.T. -0.05 min
 Lab File: BF081108.D
 Acq: 20 Aug 2015 5:11

Tgt Ion: 264 Resp: 158927
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.6 29.4
 265 22.0 17.5 26.3

