

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081915\
 Data File : BF081122.D
 Acq On : 20 Aug 2015 12:24
 Operator : UM/IZ
 Sample : G3230-02 5X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB2A

Quant Time: Aug 20 13:07:32 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 20 11:22:13 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	73063	20.00	ng	0.00
21) Naphthalene-d8	7.88	136	319444	20.00	ng	0.00
38) Acenaphthene-d10	9.62	164	128419	20.00	ng	0.00
63) Phenanthrene-d10	11.09	188	223250	20.00	ng	0.00
75) Chrysene-d12	13.72	240	141386	20.00	ng	0.01
86) Perylene-d12	15.07	264	113034	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.14	112	113630	23.39	ng	0.00
7) Phenol-d6	6.23	99	163897	25.86	ng	0.00
23) Nitrobenzene-d5	7.16	82	99027	14.16	ng	-0.01
41) 2,4,6-Tribromophenol	10.40	330	23674	21.27	ng	0.00
44) 2-Fluorobiphenyl	8.95	172	168585	17.20	ng	-0.01
78) Terphenyl-d14	12.68	244	116387	17.65	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081915\
Data File : BF081122.D
Acq On : 20 Aug 2015 12:24
Operator : UM/IZ
Sample : G3230-02 5X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB2A

Quant Time: Aug 20 13:07:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 20 11:22:13 2015
Response via : Initial Calibration

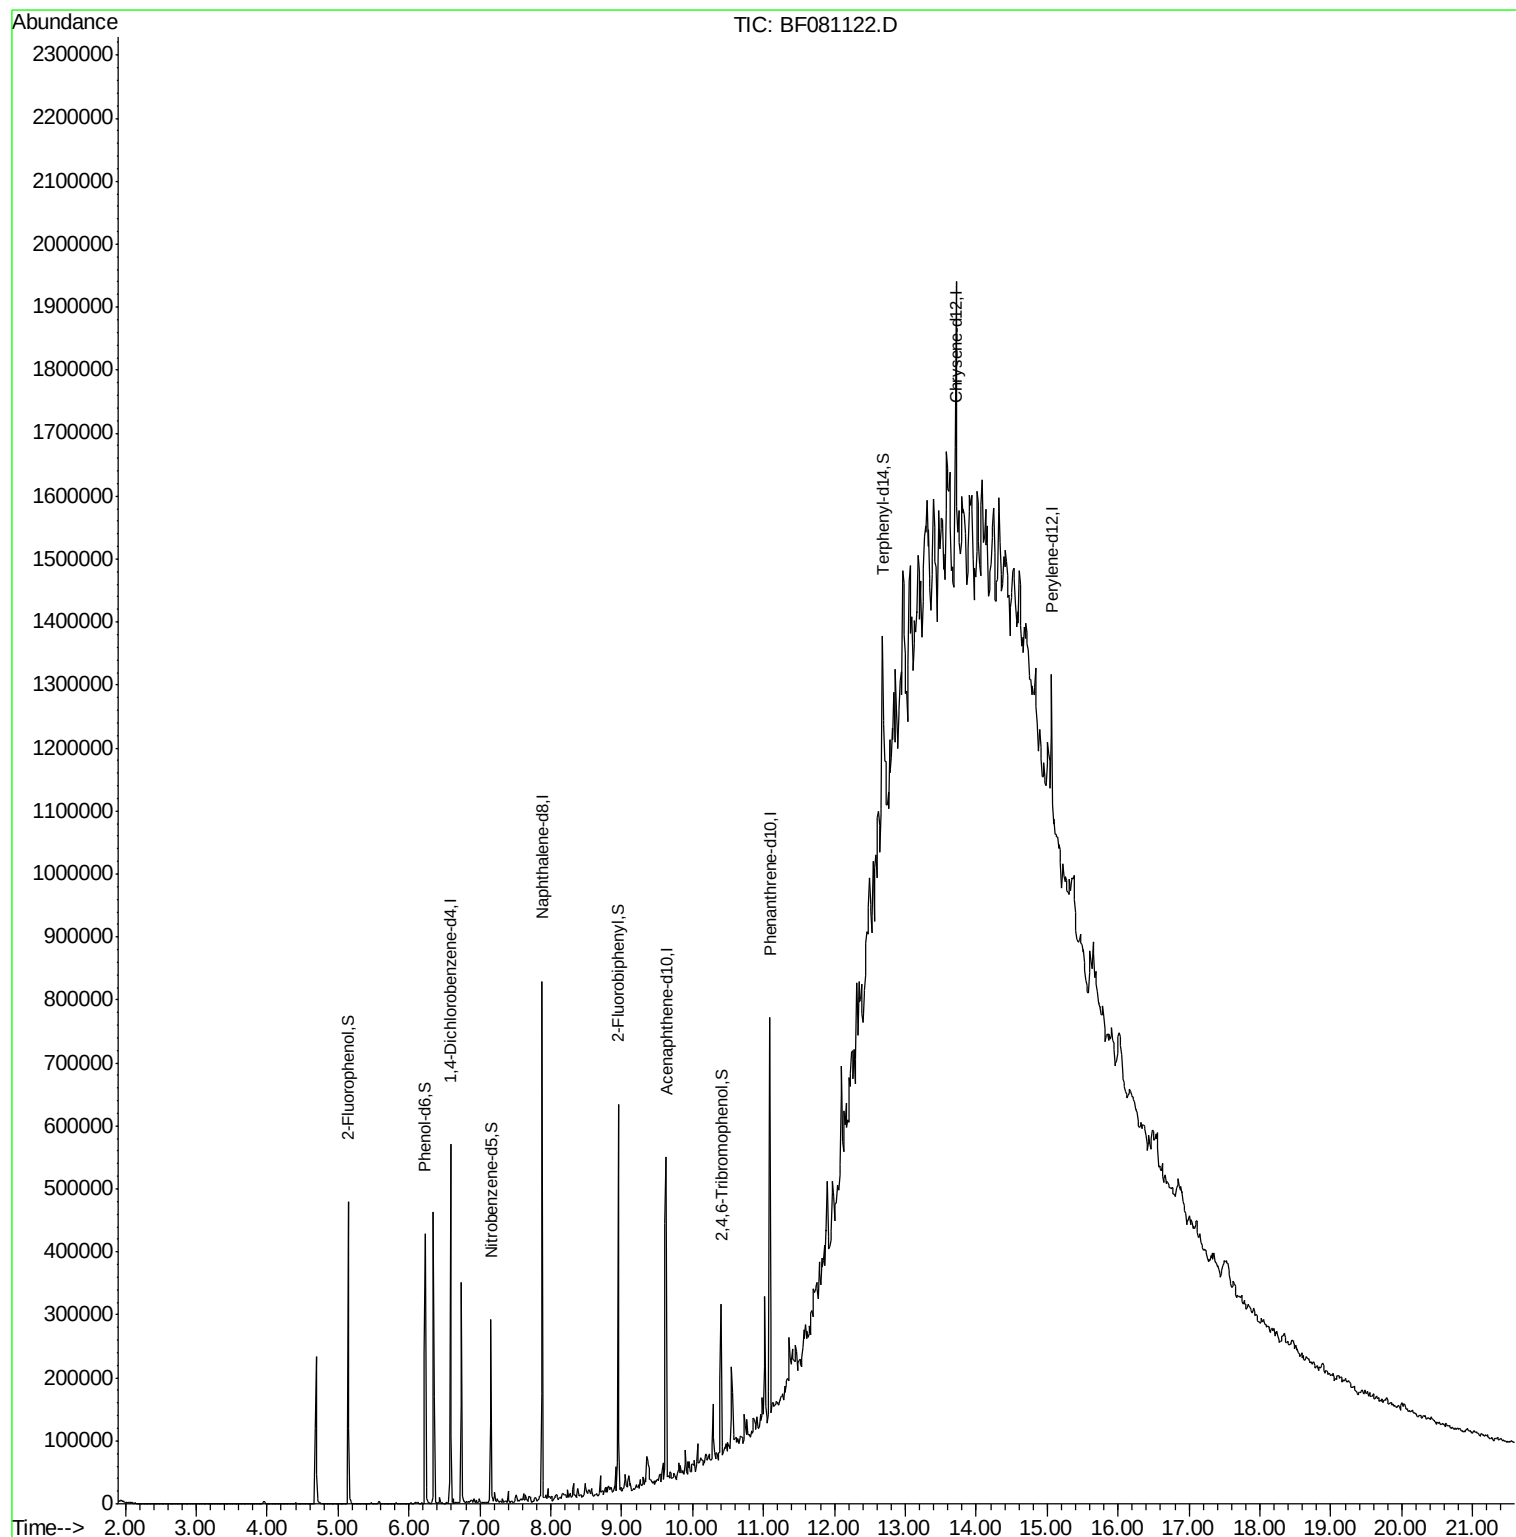

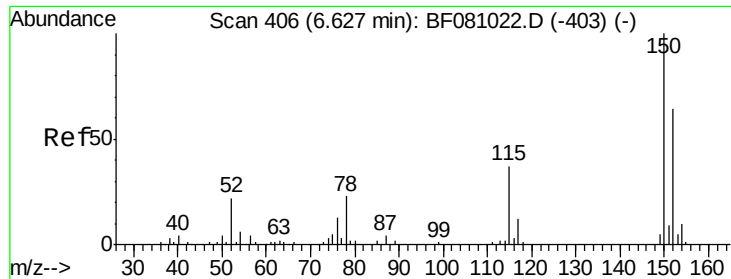


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.58 min Scan# 411
Delta R.T. -0.00 min
Lab File: BF081122.D
Acq: 20 Aug 2015 12:24

Instrument :
BNA_F
ClientSampleId :
SB2A

Tgt Ion:152 Resp: 73063
Ion Ratio Lower Upper
152 100
150 162.5 123.8 185.6
115 69.9 52.1 78.1

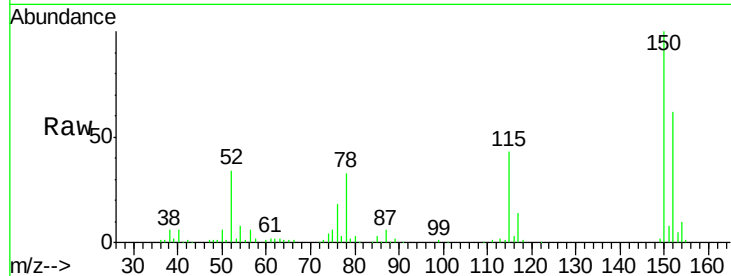


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

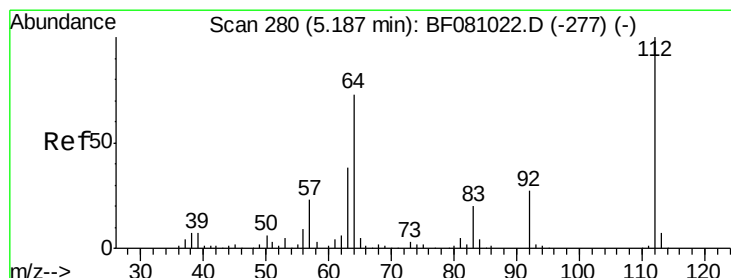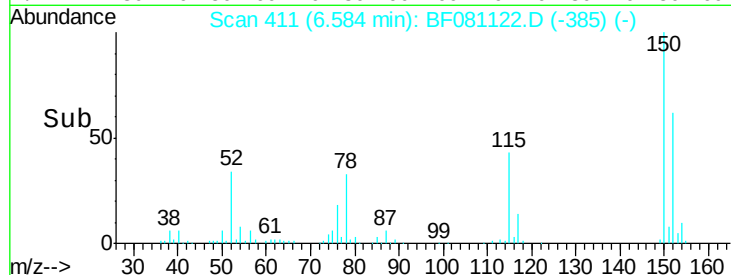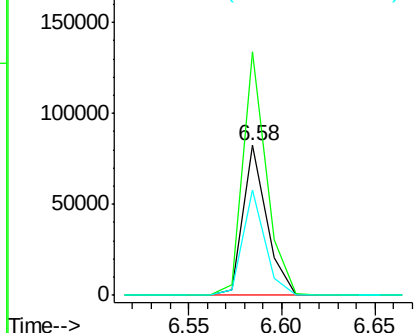



#5


2-Fluorophenol
Concen: 23.39 ng
RT: 5.14 min Scan# 285
Delta R.T. -0.00 min
Lab File: BF081122.D
Acq: 20 Aug 2015 12:24

Tgt Ion:112 Resp: 113630
Ion Ratio Lower Upper
112 100
64 79.0 66.9 100.3
63 40.6 38.1 57.1

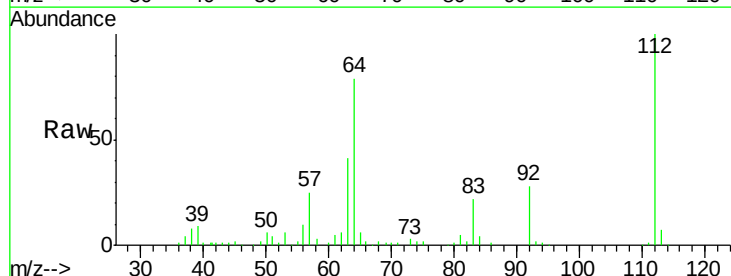

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

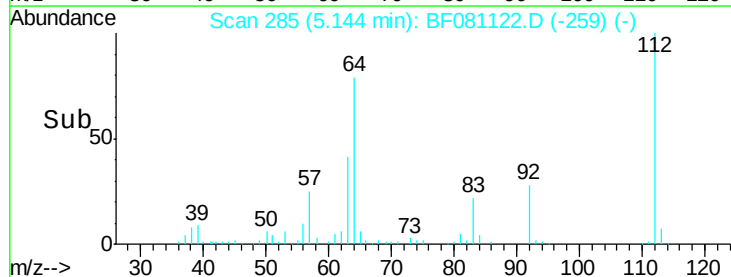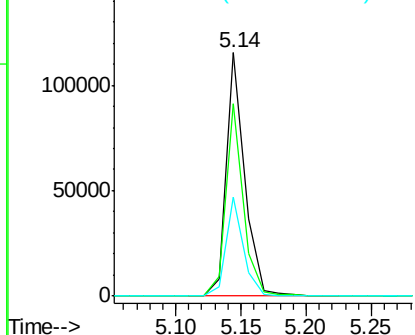

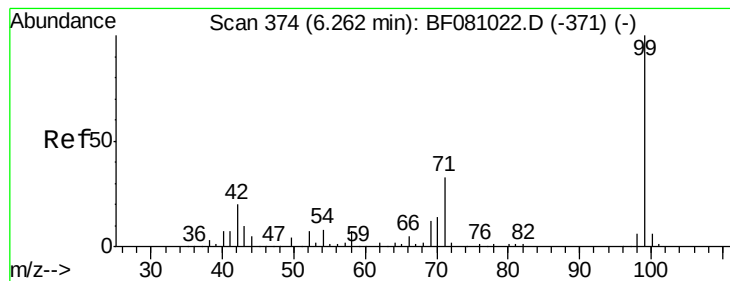

#7

Phenol-d6

Concen: 25.86 ng

RT: 6.23 min Scan# 380

Delta R.T. -0.00 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24

Instrument :

BNA_F

ClientSampleId :

SB2A


Tgt Ion: 99 Resp: 163897

Ion Ratio Lower Upper

99 100

42 18.4 19.6 29.4#




71 31.9 31.2 46.8

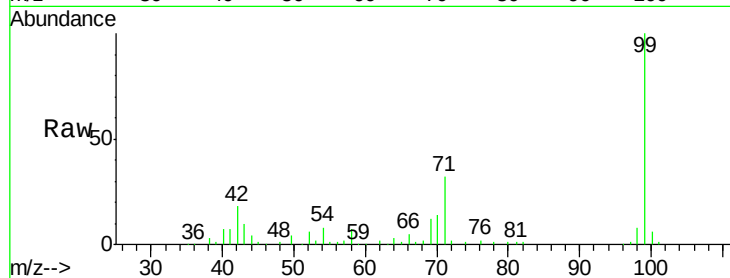

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

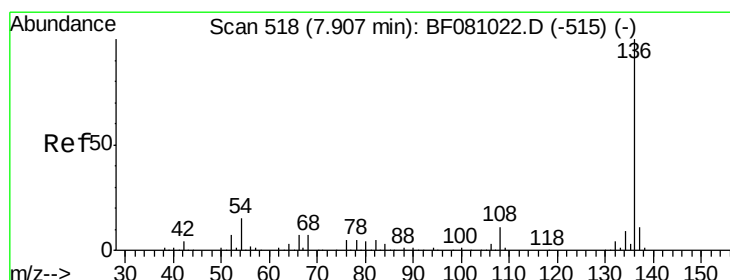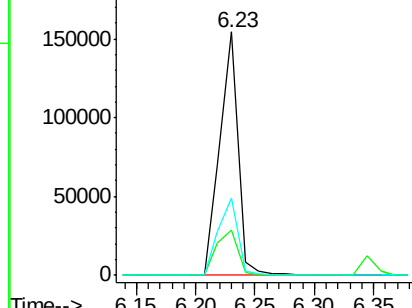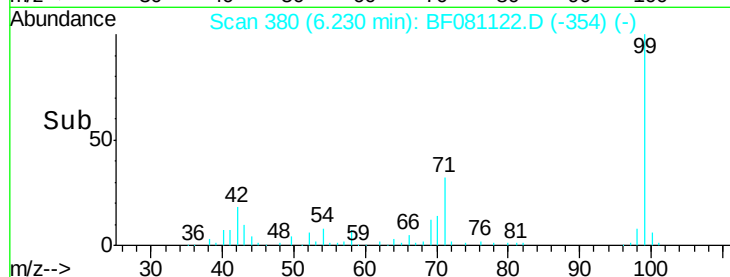

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.88 min Scan# 524

Delta R.T. -0.00 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24

Tgt Ion: 136 Resp: 319444


Ion Ratio Lower Upper

136 100

137 10.9 8.2 12.2

54 10.4 7.7 11.5

68 5.5 3.4 5.2#


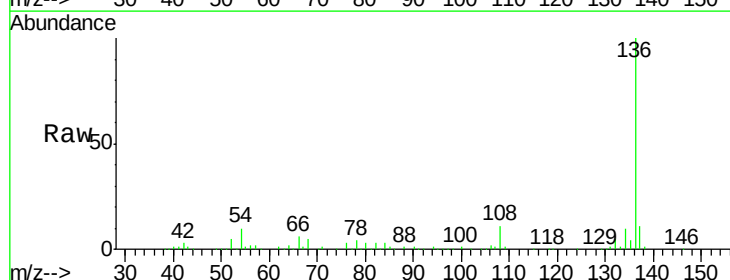



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

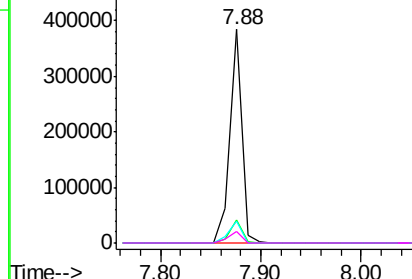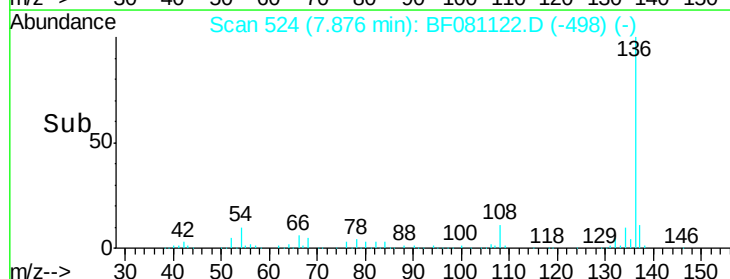


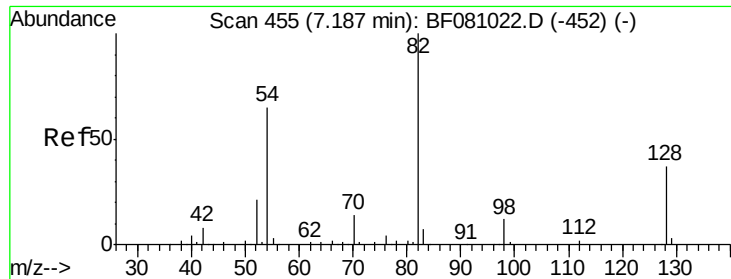




#23
 Nitrobenzene-d5
 Concen: 14.16 ng
 RT: 7.16 min Scan# 461
 Delta R.T. -0.01 min
 Lab File: BF081122.D
 Acq: 20 Aug 2015 12:24

Instrument :
 BNA_F
 ClientSampleId :
 SB2A

Tgt Ion: 82 Resp: 99027
 Ion Ratio Lower Upper
 82 100
 128 44.3 28.6 42.8#
 54 55.7 55.1 82.7

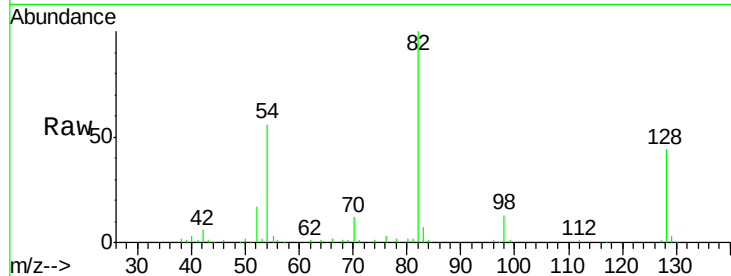


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

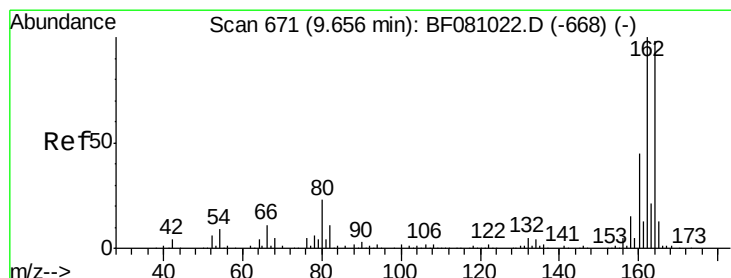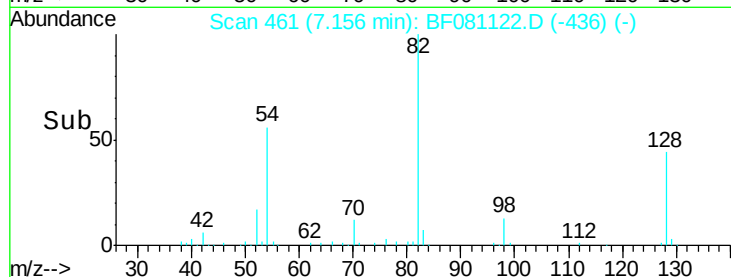
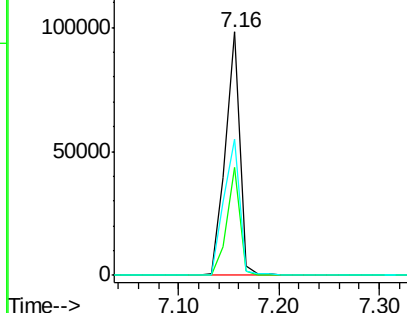



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.62 min Scan# 677
 Delta R.T. -0.00 min
 Lab File: BF081122.D
 Acq: 20 Aug 2015 12:24

Tgt Ion: 164 Resp: 128419
 Ion Ratio Lower Upper
 164 100
 162 105.5 83.8 125.8
 160 49.9 39.8 59.8

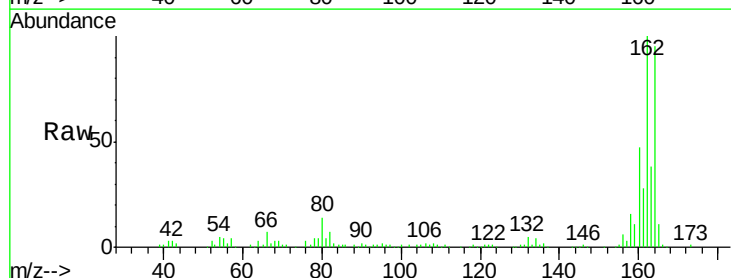

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

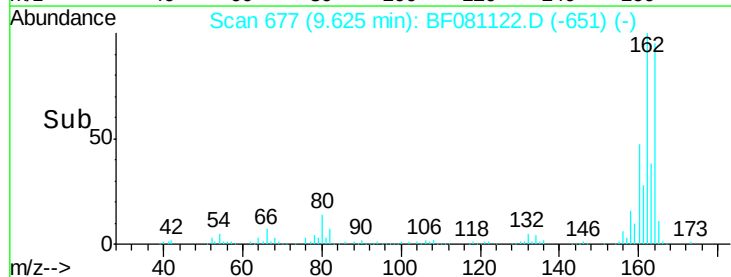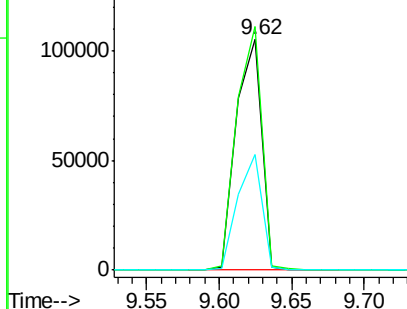

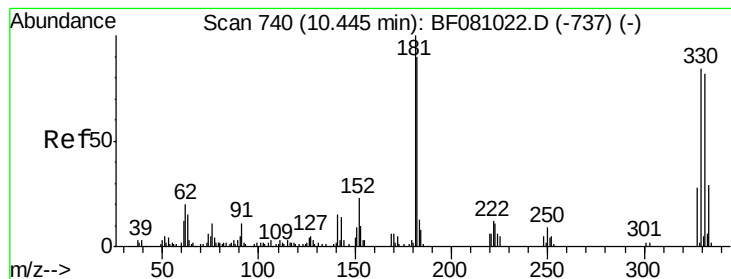

#41

2,4,6-Tribromophenol

Concen: 21.27 ng

RT: 10.40 min Scan# 745

Delta R.T. -0.00 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24

Instrument :

BNA_F

ClientSampleId :

SB2A


Tgt Ion:330 Resp: 23674

Ion Ratio Lower Upper

330 100

332 97.1 77.3 115.9




141 51.1 44.9 67.3

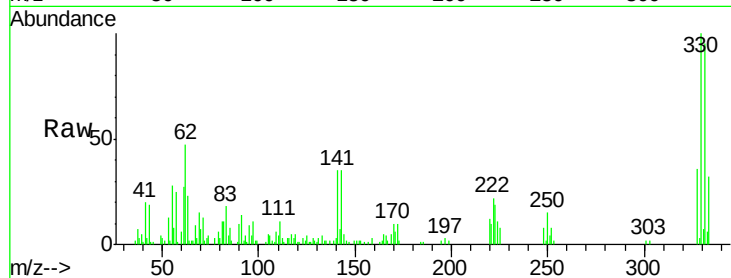

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

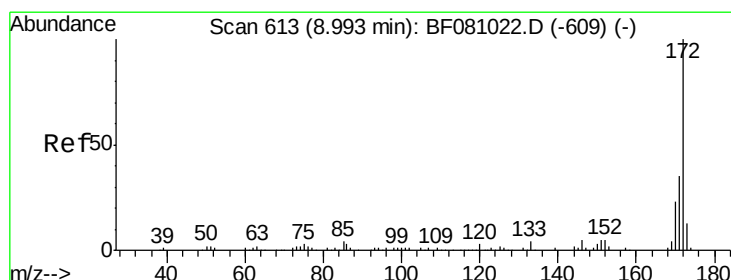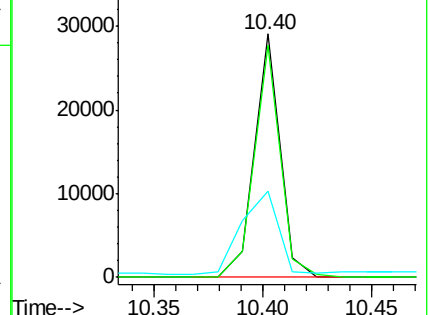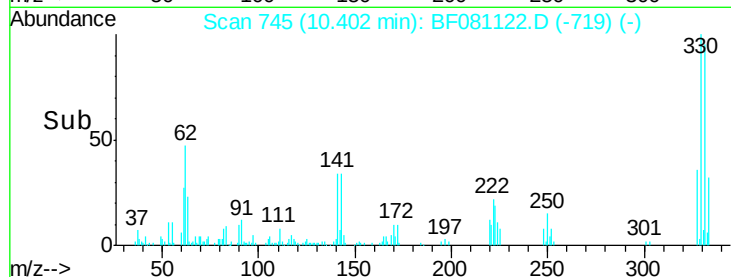

#44

2-Fluorobiphenyl

Concen: 17.20 ng

RT: 8.95 min Scan# 618

Delta R.T. -0.01 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24


Tgt Ion:172 Resp: 168585

Ion Ratio Lower Upper

172 100

171 34.9 28.9 43.3



170 23.3 19.4 29.2

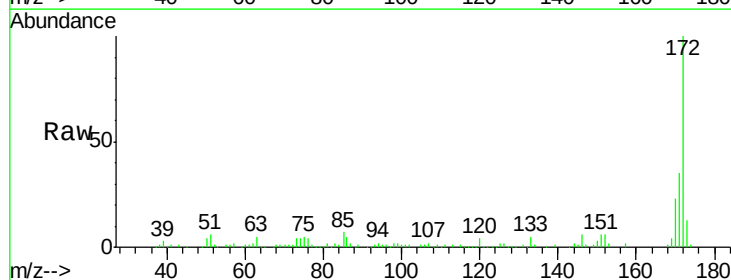


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

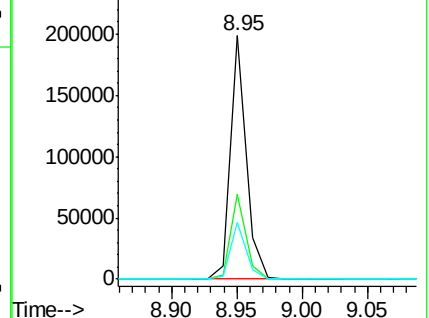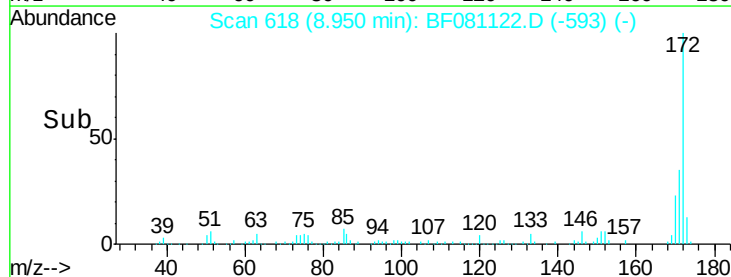

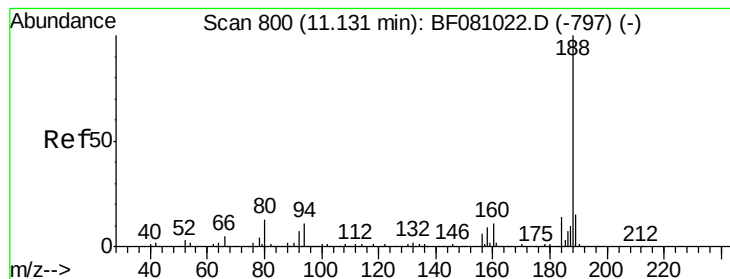

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.09 min Scan# 805

Delta R.T. -0.00 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24

Instrument :

BNA_F

ClientSampleId :

SB2A


Tgt Ion:188 Resp: 223250

Ion Ratio Lower Upper

188 100

94 11.2 8.2 12.2




80 13.9 9.5 14.3

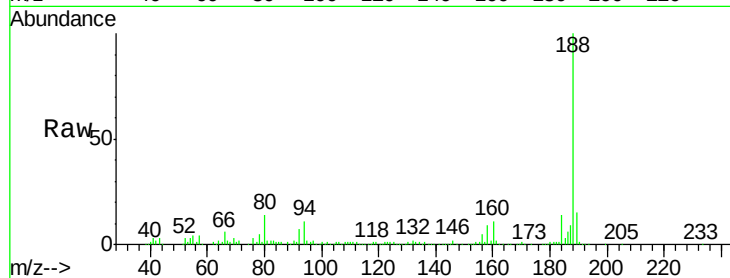

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

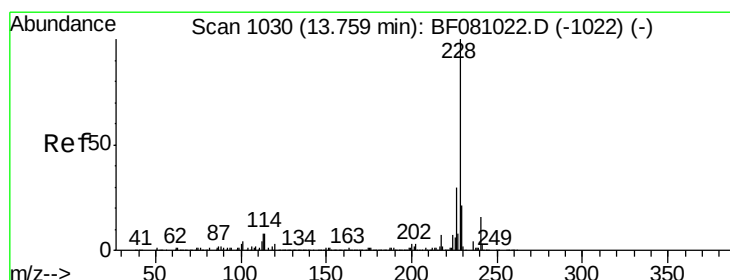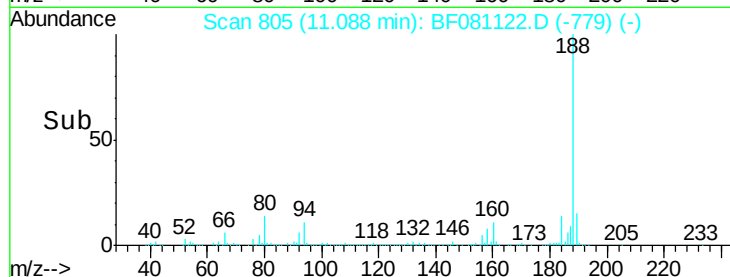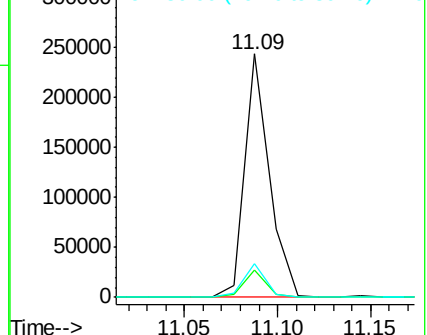

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.72 min Scan# 1035

Delta R.T. 0.01 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24


Tgt Ion:240 Resp: 141386

Ion Ratio Lower Upper

240 100

120 11.9 5.6 8.4#



236 27.0 20.6 30.8

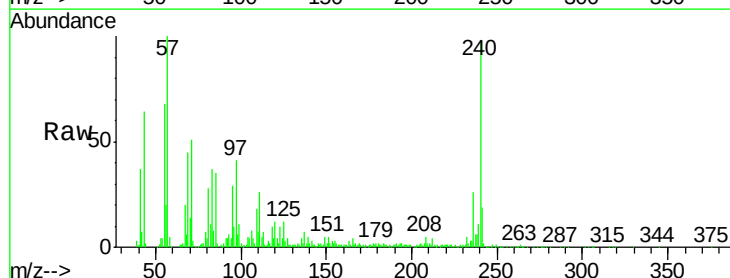


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

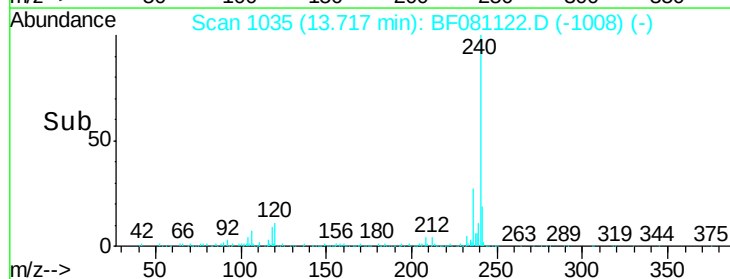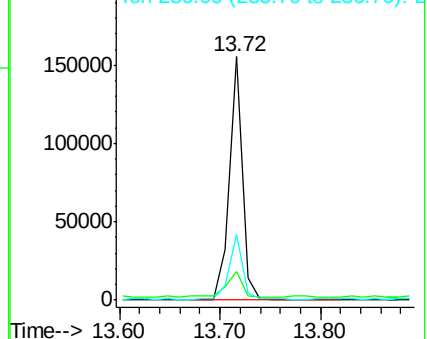

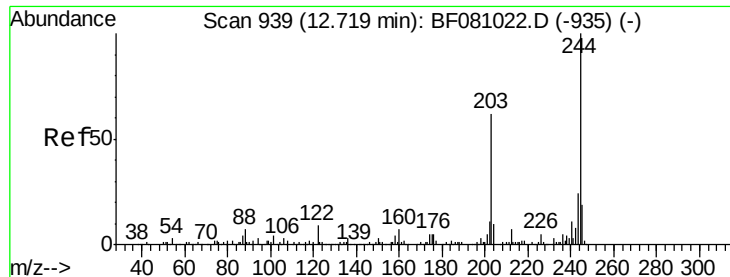

#78

Terphenyl-d14

Concen: 17.65 ng

RT: 12.68 min Scan# 944

Delta R.T. -0.00 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24

Instrument :

BNA_F

ClientSampleId :

SB2A


Tgt Ion:244 Resp: 116387

Ion Ratio Lower Upper

244 100

212 7.7 5.8 8.8




122 11.5 8.2 12.4

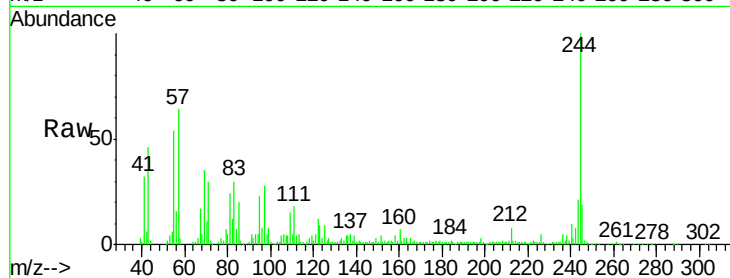

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

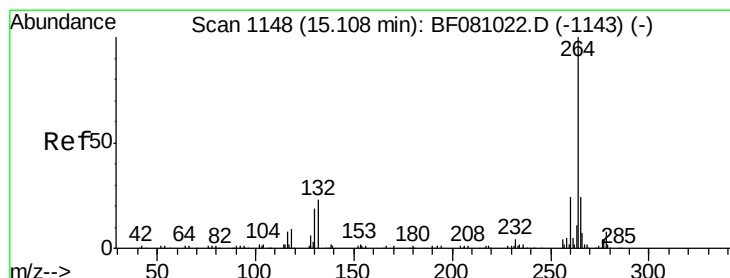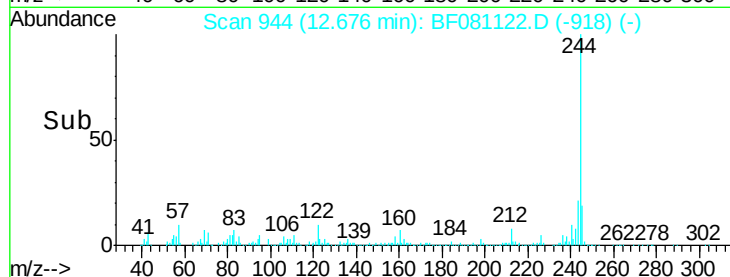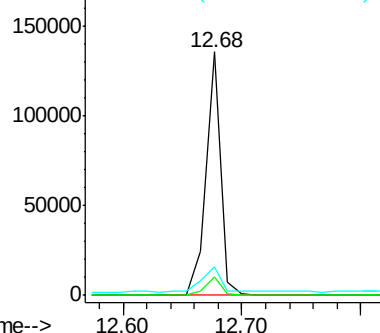

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.07 min Scan# 1153

Delta R.T. 0.02 min

Lab File: BF081122.D

Acq: 20 Aug 2015 12:24


Tgt Ion:264 Resp: 113034

Ion Ratio Lower Upper

264 100

260 24.4 19.6 29.4

265 22.5 17.5 26.3

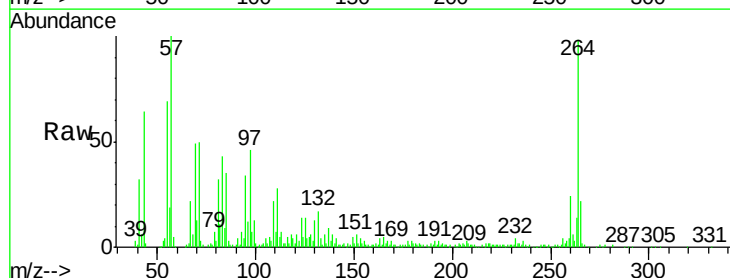

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

