


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081915\
 Data File : BF081082.D
 Acq On : 19 Aug 2015 14:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 20 11:22:13 2015

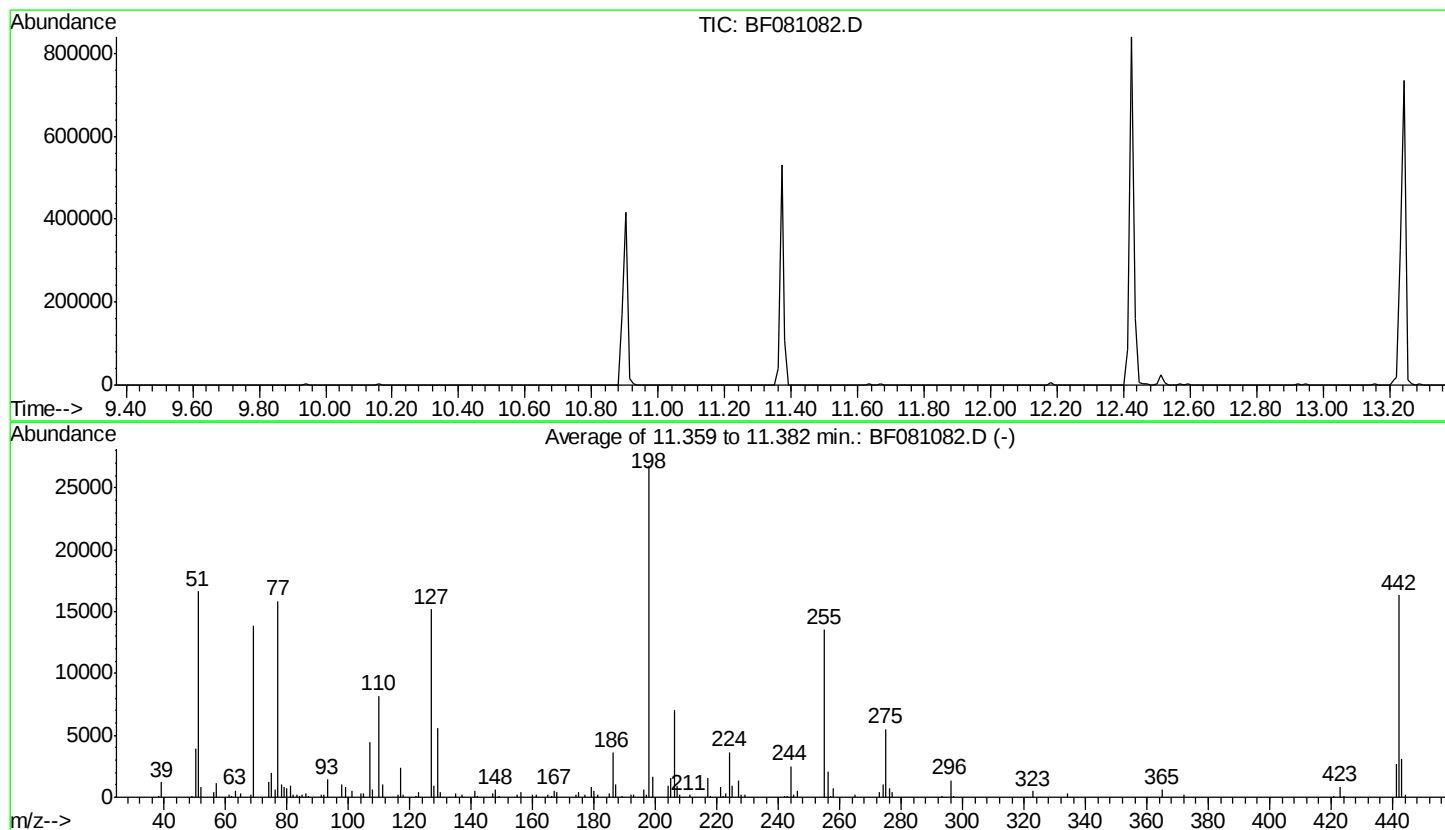

AutoFind: Scans 820, 821, 822; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.1	16628	PASS
68	69	0.00	2	1.4	197	PASS
69	198	0.00	100	51.6	13829	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.7	15193	PASS
197	198	0.00	2	0.6	165	PASS
198	198	100	100	100.0	26782	PASS
199	198	5	9	6.4	1704	PASS
275	198	10	60	20.6	5509	PASS
365	198	1	100	2.1	572	PASS
441	442	0.01	24	16.6	2705	PASS
442	198	50	100	60.9	16312	PASS
443	442	15	24	19.3	3147	PASS