
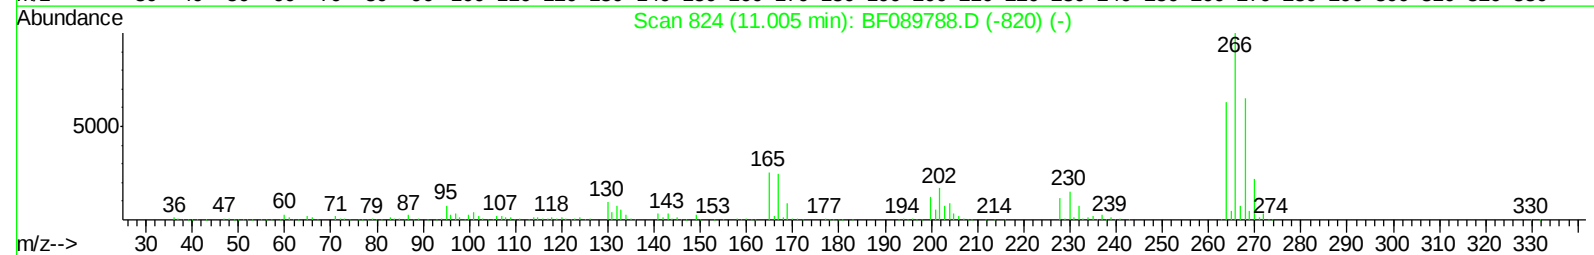
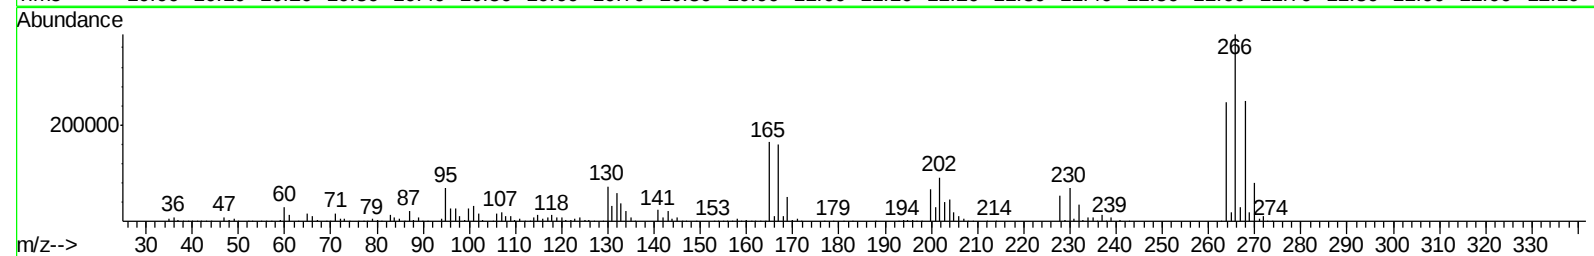


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081916\
Data File : BF089783.D
Acq On : 19 Aug 2016 9:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:02:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 01:47:27 2016
Response via : Initial Calibration

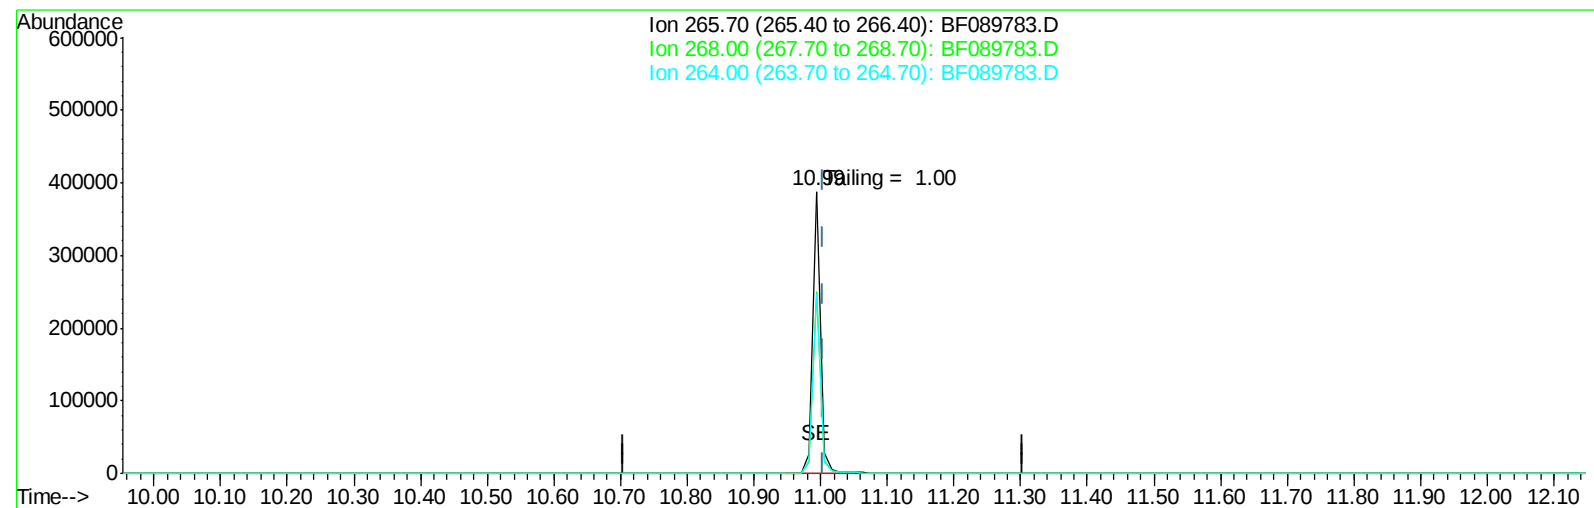

TIC: BF089783.D

(69) Pentachlorophenol (C)




10.994min (-0.011) 14967.72ng

response 314968

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	64.63
264.00	63.90	63.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081916\
Data File : BF089783.D
Acq On : 19 Aug 2016 9:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:02:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 01:47:27 2016
Response via : Initial Calibration

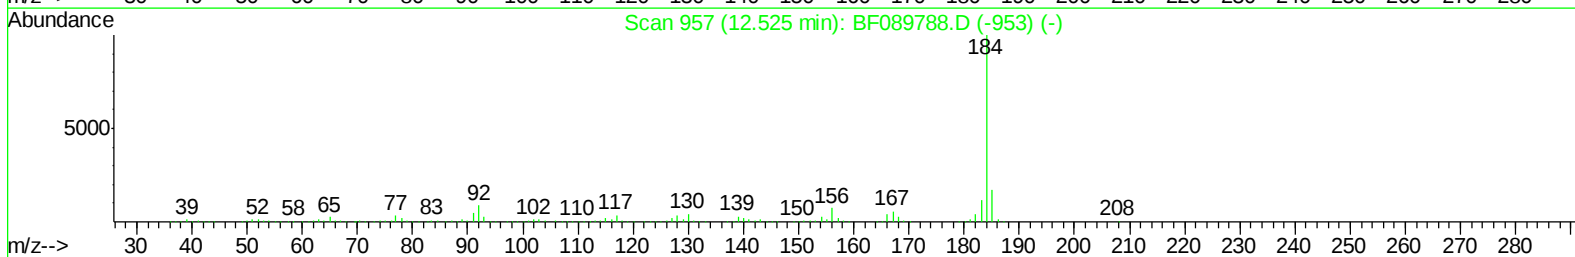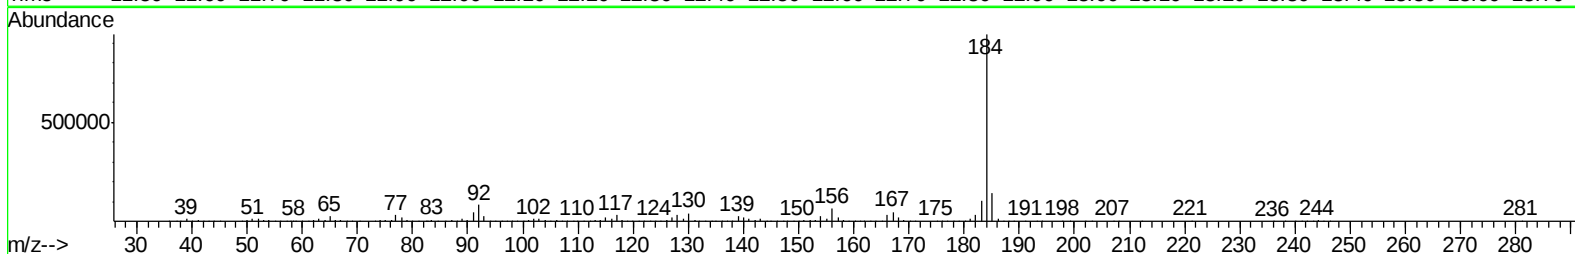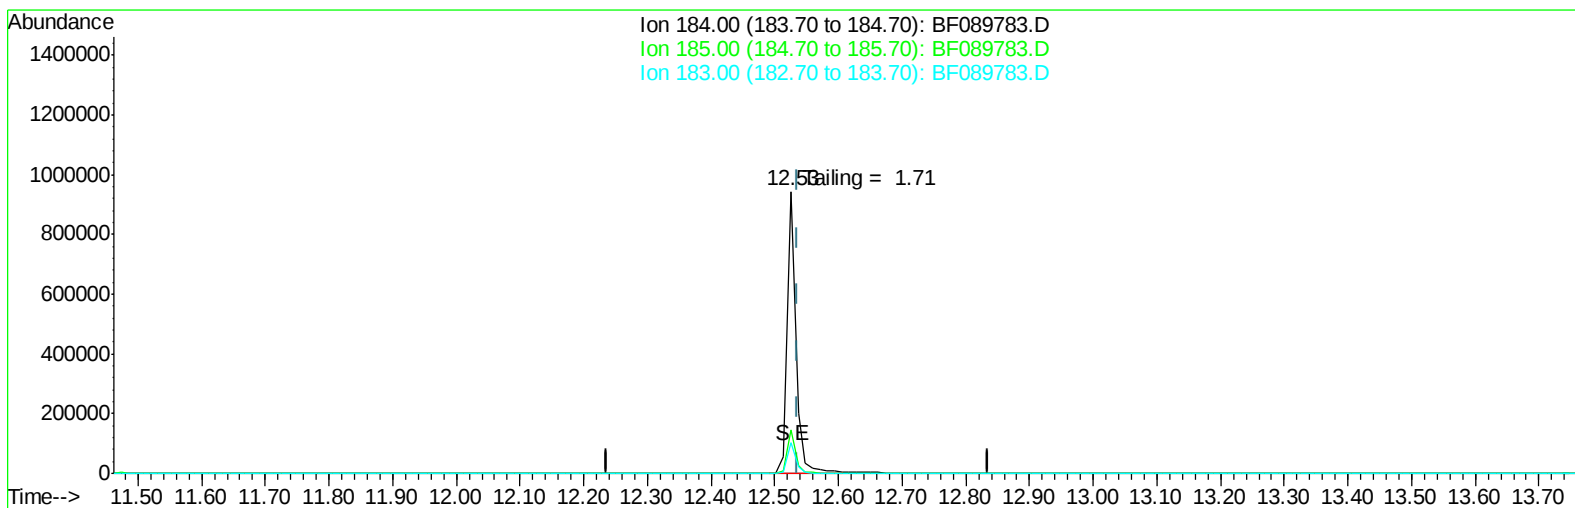

TIC: BF089783.D

(76) Benzidine

12.525min (-0.011) 4746.85ng

response 906344

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	15.29
183.00	12.10	10.90
0.00	0.00	0.00