
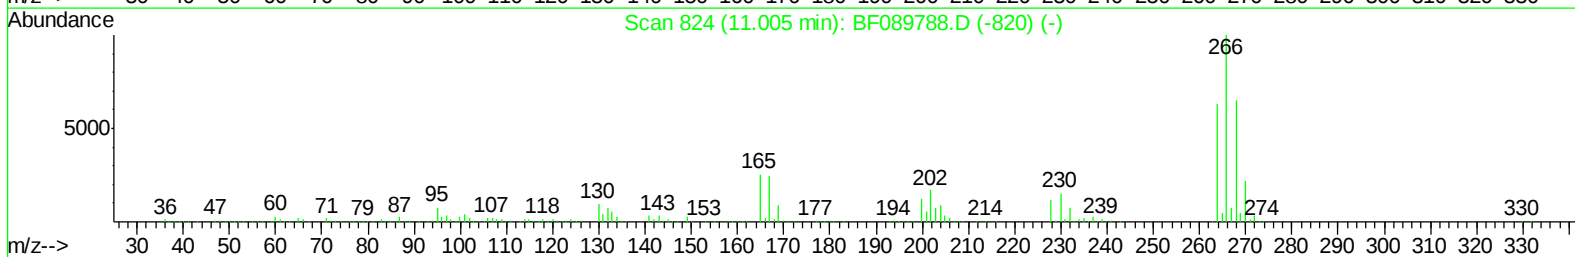
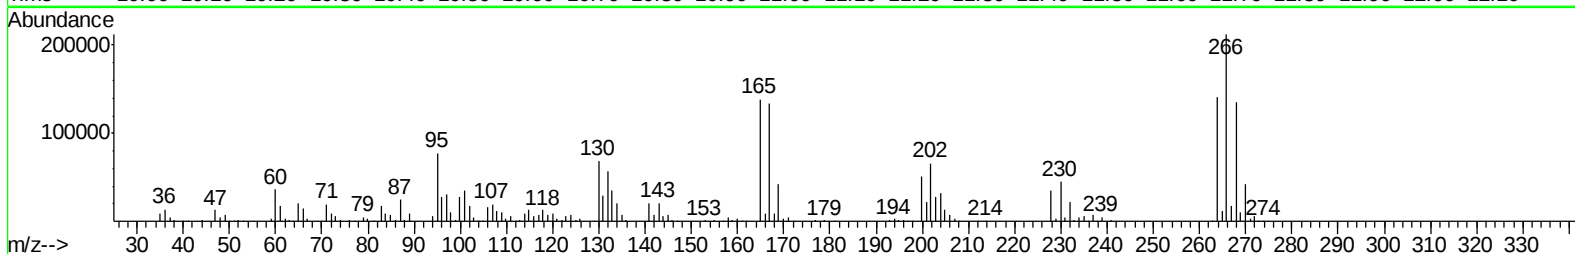


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081916\
Data File : BF089793.D
Acq On : 19 Aug 2016 14:09
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 06:03:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 01:47:27 2016
Response via : Initial Calibration

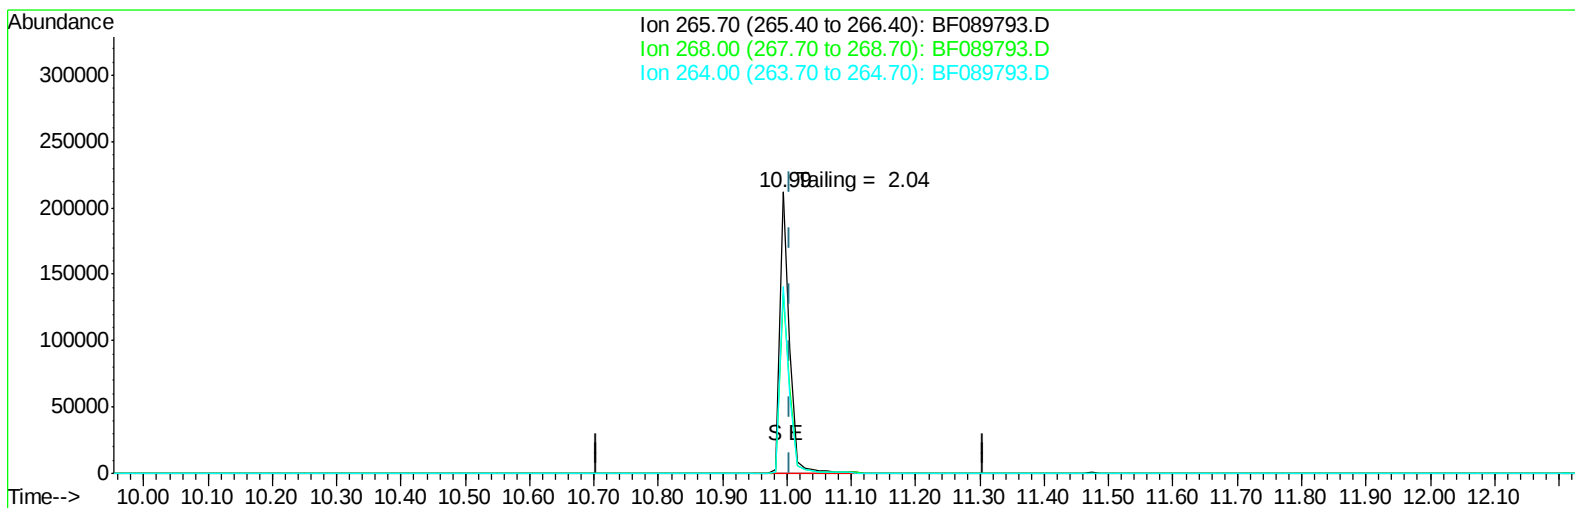

TIC: BF089793.D

(69) Pentachlorophenol (C)




10.993min (-0.011) 97438.33ng

response 230539

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	63.77
264.00	63.90	66.37
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081916\  
Data File : BF089793.D  
Acq On    : 19 Aug 2016  14:09  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Aug 22 06:03:27 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 01:47:27 2016
Response via : Initial Calibration

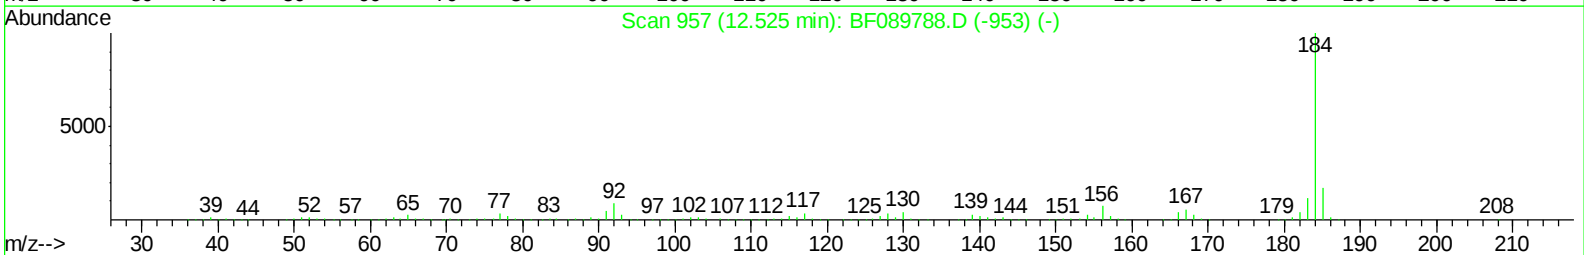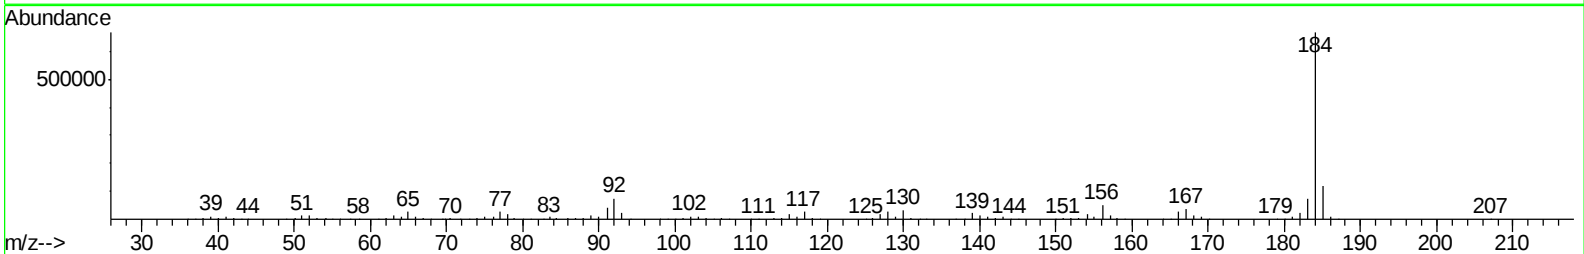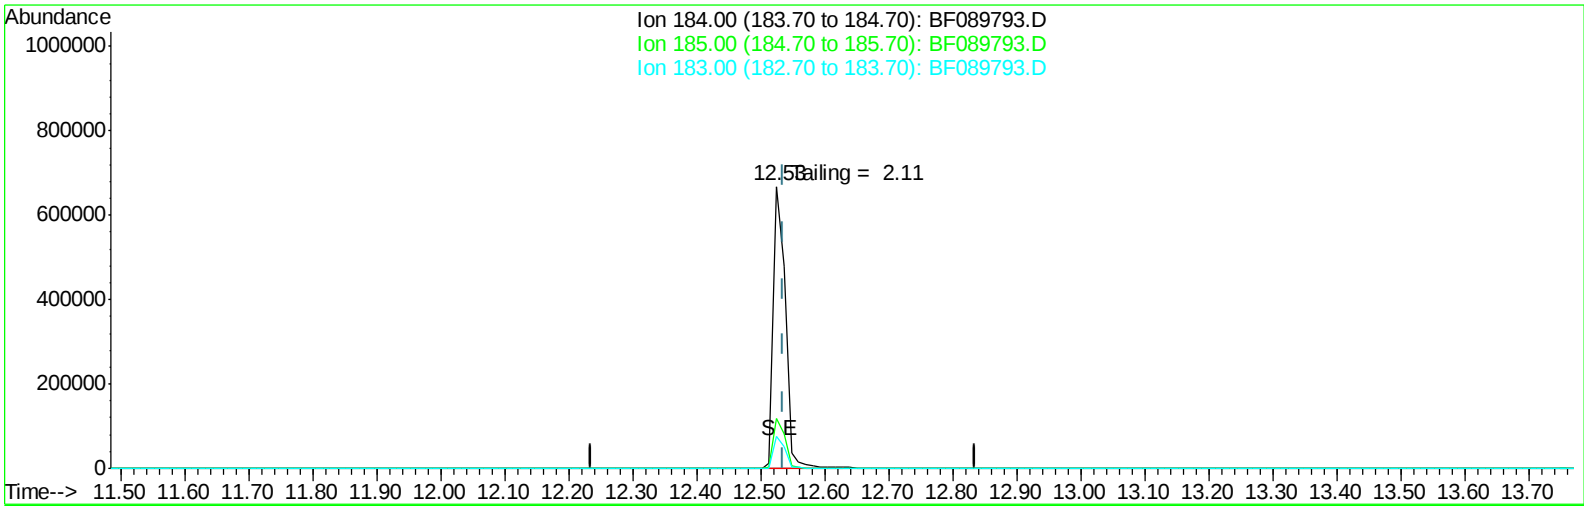

TIC: BF089793.D

(76) Benzidine

12.525min (-0.011) 67893.77ng

response 859097

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	17.55
183.00	12.10	11.20
0.00	0.00	0.00