


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081916\
 Data File : BF089783.D
 Acq On : 19 Aug 2016 9:02
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

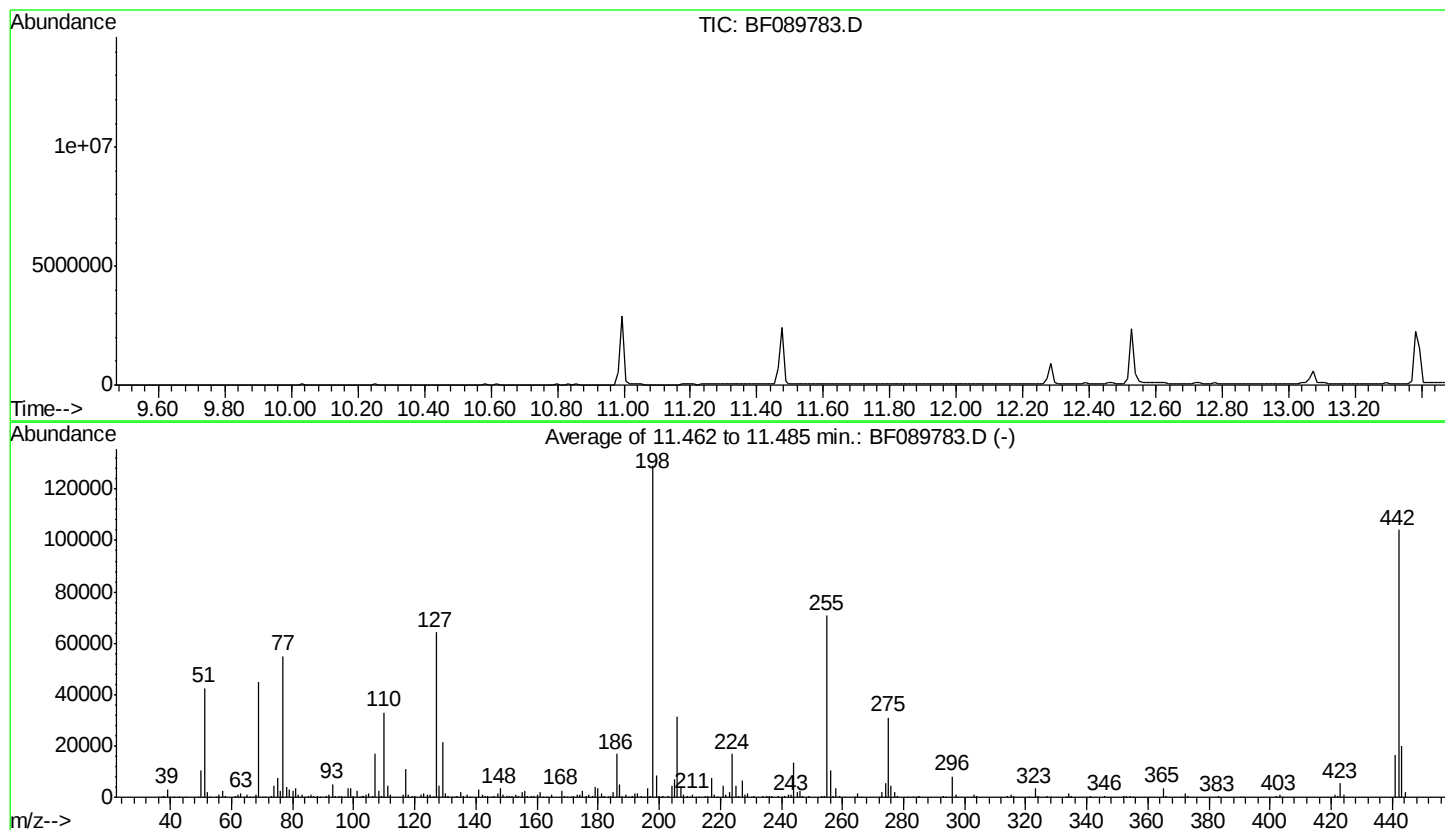

AutoFind: Scans 864, 865, 866; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	42512	PASS
68	69	0.00	2	1.9	852	PASS
69	198	0.00	100	34.7	44760	PASS
70	69	0.00	2	0.2	107	PASS
127	198	10	80	49.7	64191	PASS
197	198	0.00	2	0.5	611	PASS
198	198	100	100	100.0	129171	PASS
199	198	5	9	6.5	8334	PASS
275	198	10	60	24.0	31030	PASS
365	198	1	100	2.8	3677	PASS
441	442	0.01	24	15.8	16430	PASS
442	198	50	100	80.5	103999	PASS
443	442	15	24	19.0	19741	PASS