


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081916\
 Data File : BF089793.D
 Acq On : 19 Aug 2016 14:09
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

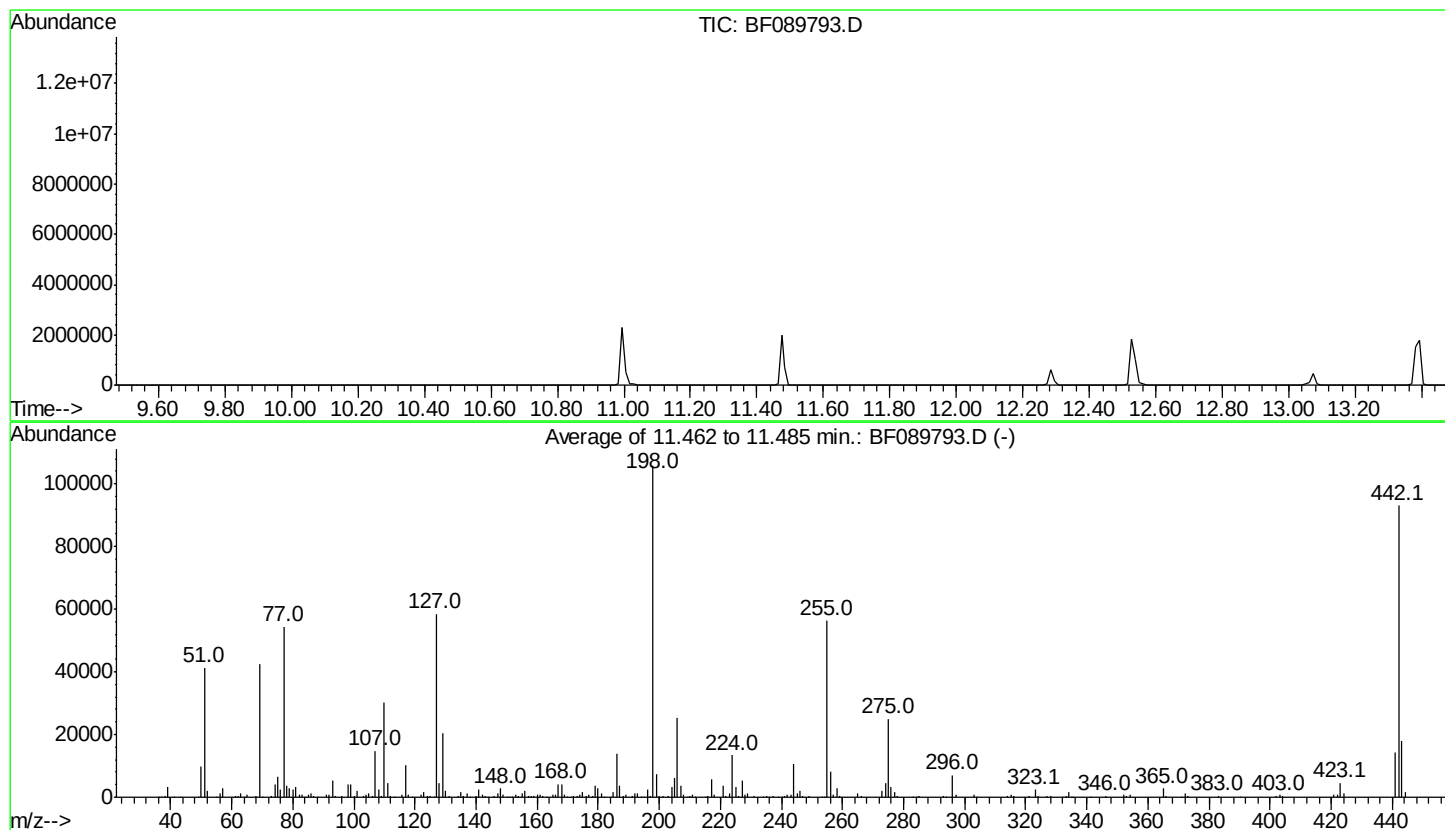

AutoFind: Scans 864, 865, 866; Background Corrected with Scan 861

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	41427	PASS
68	69	0.00	2	1.5	624	PASS
69	198	0.00	100	40.1	42441	PASS
70	69	0.00	2	0.5	215	PASS
127	198	10	80	55.3	58470	PASS
197	198	0.00	2	0.3	312	PASS
198	198	100	100	100.0	105786	PASS
199	198	5	9	6.9	7319	PASS
275	198	10	60	23.6	24952	PASS
365	198	1	100	2.7	2856	PASS
441	442	0.01	24	15.4	14281	PASS
442	198	50	100	87.9	93026	PASS
443	442	15	24	19.6	18187	PASS