
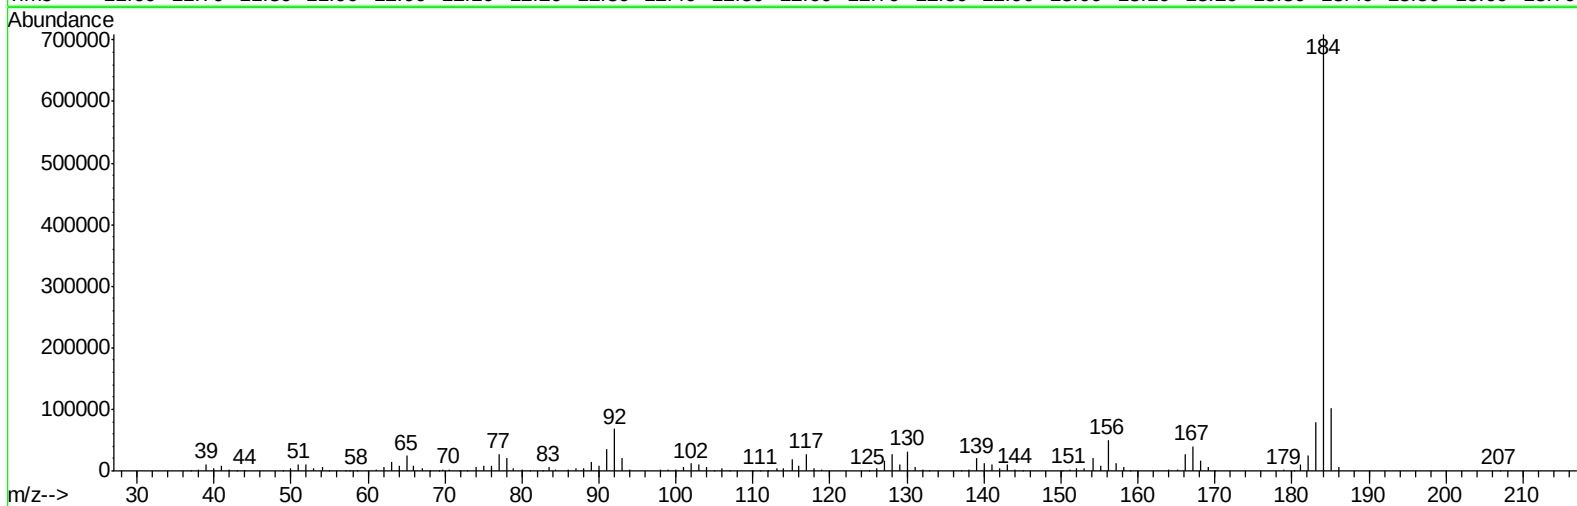


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081917\
 Data File : BF097871.D
 Acq On : 19 Aug 2017 11:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 05:11:46 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 13:25:08 2017
 Response via : Initial Calibration

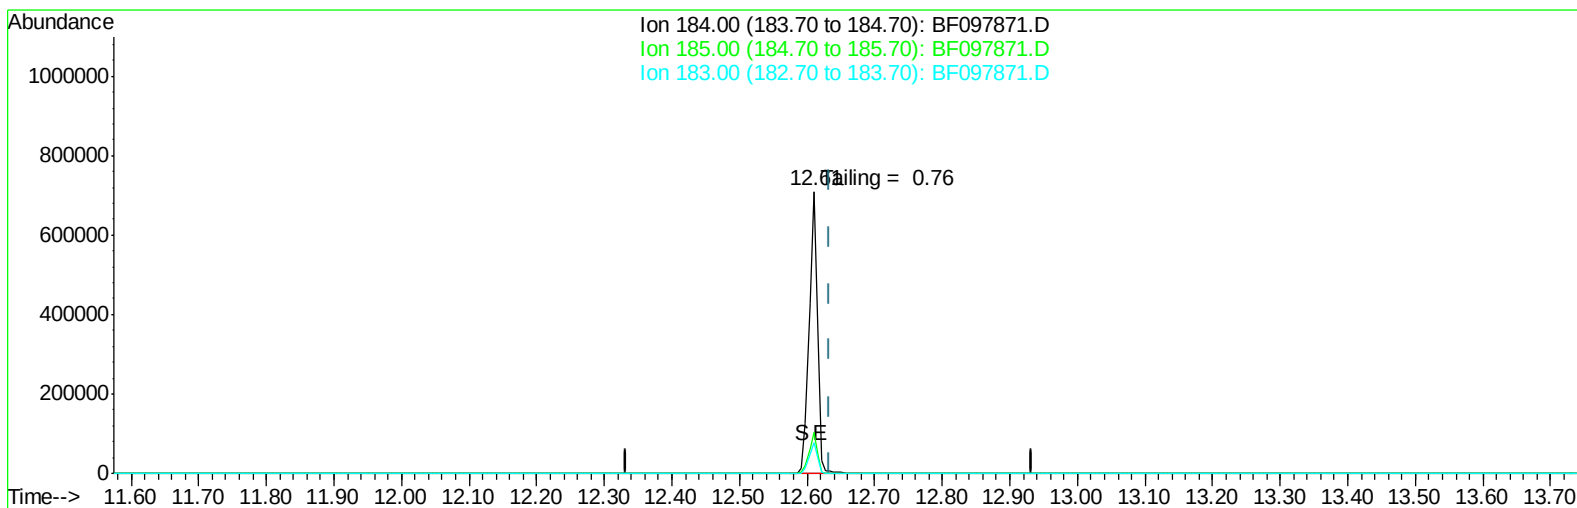

TIC: BF097871.D

(76) Benzidine



12.610min (-0.023) 2511.57ng

response 600981

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.43#
183.00	12.20	11.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081917\
Data File : BF097871.D
Acq On : 19 Aug 2017 11:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 05:11:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

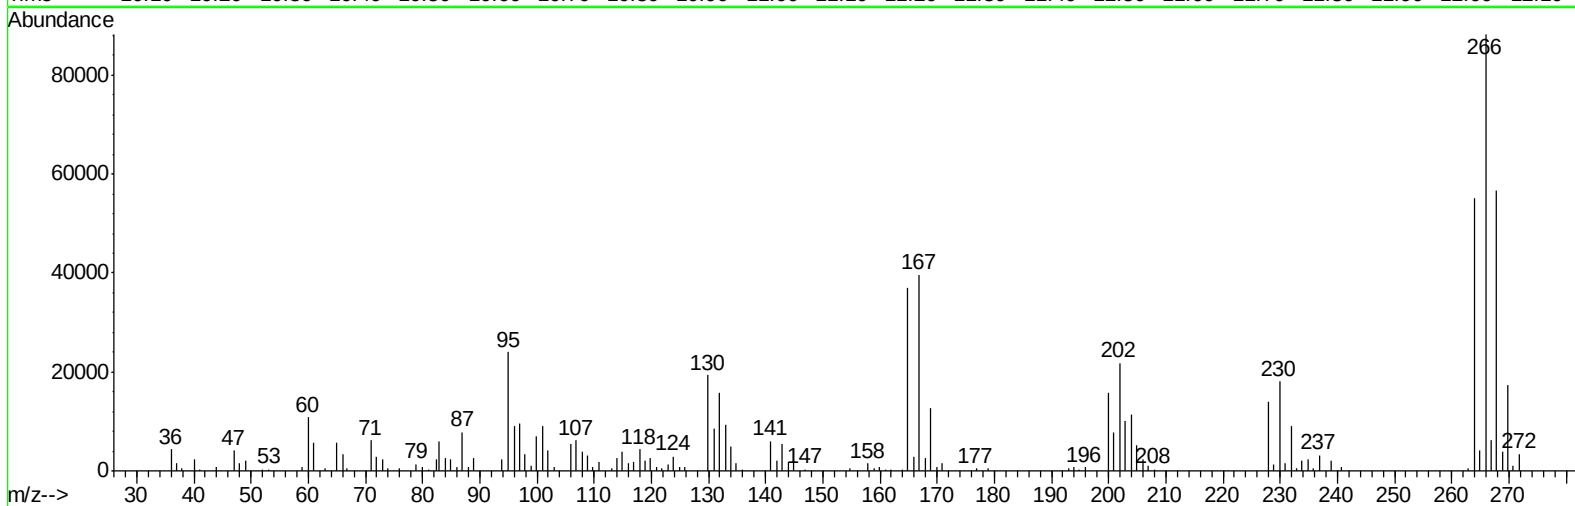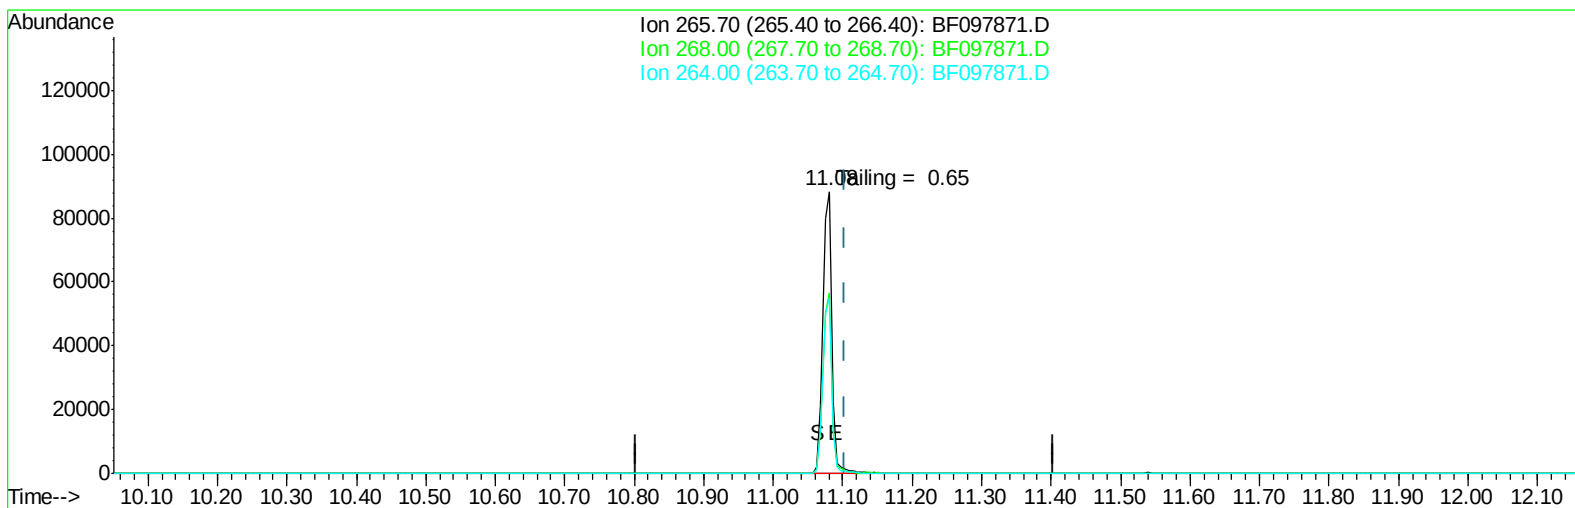

TIC: BF097871.D

(69) Pentachlorophenol (C)

11.080min (-0.023) 1088.00ng

response 78988

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.11
264.00	64.60	62.35
0.00	0.00	0.00