

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081917\
 Data File : BF097890.D
 Acq On : 19 Aug 2017 20:32
 Operator : SJ/JU
 Sample : I4847-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PVSC-A-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.940	482	485	494	rVB	123770	124142	9.64%	0.927%
2	5.357	552	556	560	rVB	863065	734935	57.07%	5.490%
3	6.381	726	730	739	rVB	923129	813567	63.17%	6.078%
4	6.522	750	754	758	rBV	994253	818608	63.56%	6.115%
5	6.757	790	794	798	rBV	1059237	981295	76.20%	7.330%
6	6.916	817	821	824	rBV	684587	575927	44.72%	4.302%
7	7.316	882	889	893	rBV	542901	491644	38.18%	3.673%
8	7.363	893	897	900	rVB2	12406	16164	1.26%	0.121%
9	8.045	1008	1013	1016	rBV	1519203	1287856	100.00%	9.621%
10	9.116	1191	1195	1201	rBV	1044544	809935	62.89%	6.050%
11	9.204	1204	1210	1215	rBV2	26129	31690	2.46%	0.237%
12	9.451	1250	1252	1255	rBV2	19433	19505	1.51%	0.146%
13	9.510	1259	1262	1266	rVV	116568	99261	7.71%	0.741%
14	9.733	1298	1300	1304	rVB	30311	22724	1.76%	0.170%
15	9.792	1304	1310	1314	rBV	1306632	1244449	96.63%	9.296%
16	9.828	1314	1316	1319	rVB	24076	21259	1.65%	0.159%
17	9.998	1342	1345	1347	rVB3	21753	19809	1.54%	0.148%
18	10.233	1381	1385	1387	rVB2	30444	27574	2.14%	0.206%
19	10.339	1400	1403	1409	rVB2	27432	29609	2.30%	0.221%
20	10.451	1419	1422	1424	rBV	26860	23603	1.83%	0.176%
21	10.575	1439	1443	1448	rBV	413563	366096	28.43%	2.735%
22	10.704	1462	1465	1472	rVB2	53485	65108	5.06%	0.486%
23	10.886	1492	1496	1499	rBV4	12142	17848	1.39%	0.133%
24	11.151	1539	1541	1543	rBV	36611	26535	2.06%	0.198%
25	11.180	1543	1546	1551	rVB2	22814	27630	2.15%	0.206%
26	11.275	1558	1562	1565	rBV	1222291	1090579	84.68%	8.147%
27	11.298	1565	1566	1569	rVV	207872	108652	8.44%	0.812%
28	11.345	1569	1574	1578	rVB	48046	52618	4.09%	0.393%
29	11.504	1596	1601	1603	rBV2	18696	20696	1.61%	0.155%
30	11.575	1608	1613	1616	rVV	26069	24140	1.87%	0.180%
31	11.775	1644	1647	1649	rBV	33501	27086	2.10%	0.202%
32	11.804	1649	1652	1656	rVV	48346	40682	3.16%	0.304%
33	11.845	1656	1659	1662	rVV3	15334	18700	1.45%	0.140%
34	11.886	1662	1666	1668	rVV	51710	56129	4.36%	0.419%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081917\
 Data File : BF097890.D
 Acq On : 19 Aug 2017 20:32
 Operator : SJ/JU
 Sample : I4847-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PVSC-A-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.910	1668	1670	1674	rVB2	24201	24506	1.90%	0.183%
36	11.980	1680	1682	1685	rBV2	18583	18451	1.43%	0.138%
37	12.069	1695	1697	1699	rBV	19533	16084	1.25%	0.120%
38	12.322	1737	1740	1743	rBV2	29847	29447	2.29%	0.220%
39	12.374	1743	1749	1752	rVV3	21177	35483	2.76%	0.265%
40	12.404	1752	1754	1759	rVV4	13229	15789	1.23%	0.118%
41	12.480	1764	1767	1771	rVV	210021	182921	14.20%	1.366%
42	12.527	1773	1775	1782	rVB7	19326	23229	1.80%	0.174%
43	12.710	1800	1806	1809	rBV	188698	189025	14.68%	1.412%
44	12.827	1823	1826	1828	rBV2	12728	14534	1.13%	0.109%
45	12.857	1828	1831	1835	rVV	574555	482214	37.44%	3.602%
46	12.927	1839	1843	1848	rBV6	14986	29657	2.30%	0.222%
47	13.039	1860	1862	1866	rVB	28764	25403	1.97%	0.190%
48	13.104	1869	1873	1876	rVB2	28835	28490	2.21%	0.213%
49	13.139	1876	1879	1882	rBV2	24844	26210	2.04%	0.196%
50	13.233	1892	1895	1898	rBV2	18355	20506	1.59%	0.153%
51	13.439	1928	1930	1933	rVB3	17544	15017	1.17%	0.112%
52	13.651	1962	1966	1970	rBV3	25406	36833	2.86%	0.275%
53	13.763	1982	1985	1991	rVB4	43225	59692	4.63%	0.446%
54	13.904	2004	2009	2012	rBV	884007	878836	68.24%	6.565%
55	13.927	2012	2013	2020	rVB	84383	73469	5.70%	0.549%
56	14.010	2025	2027	2031	rBV4	13982	17550	1.36%	0.131%
57	14.392	2089	2092	2097	rBV7	23594	47839	3.71%	0.357%
58	14.921	2178	2182	2185	rBV	63911	100489	7.80%	0.751%
59	15.204	2228	2230	2236	rVB	42588	50915	3.95%	0.380%
60	15.268	2237	2241	2245	rVB	49358	58431	4.54%	0.436%
61	15.327	2247	2251	2257	rBV	533423	674561	52.38%	5.039%
62	15.792	2327	2330	2336	rBV3	26820	32410	2.52%	0.242%
63	16.274	2408	2412	2416	rBV3	25801	42472	3.30%	0.317%


Sum of corrected areas: 13386518

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097890.D
Acq On : 19 Aug 2017 20:32
Operator : SJ/JU
Sample : I4847-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
PVSC-A-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

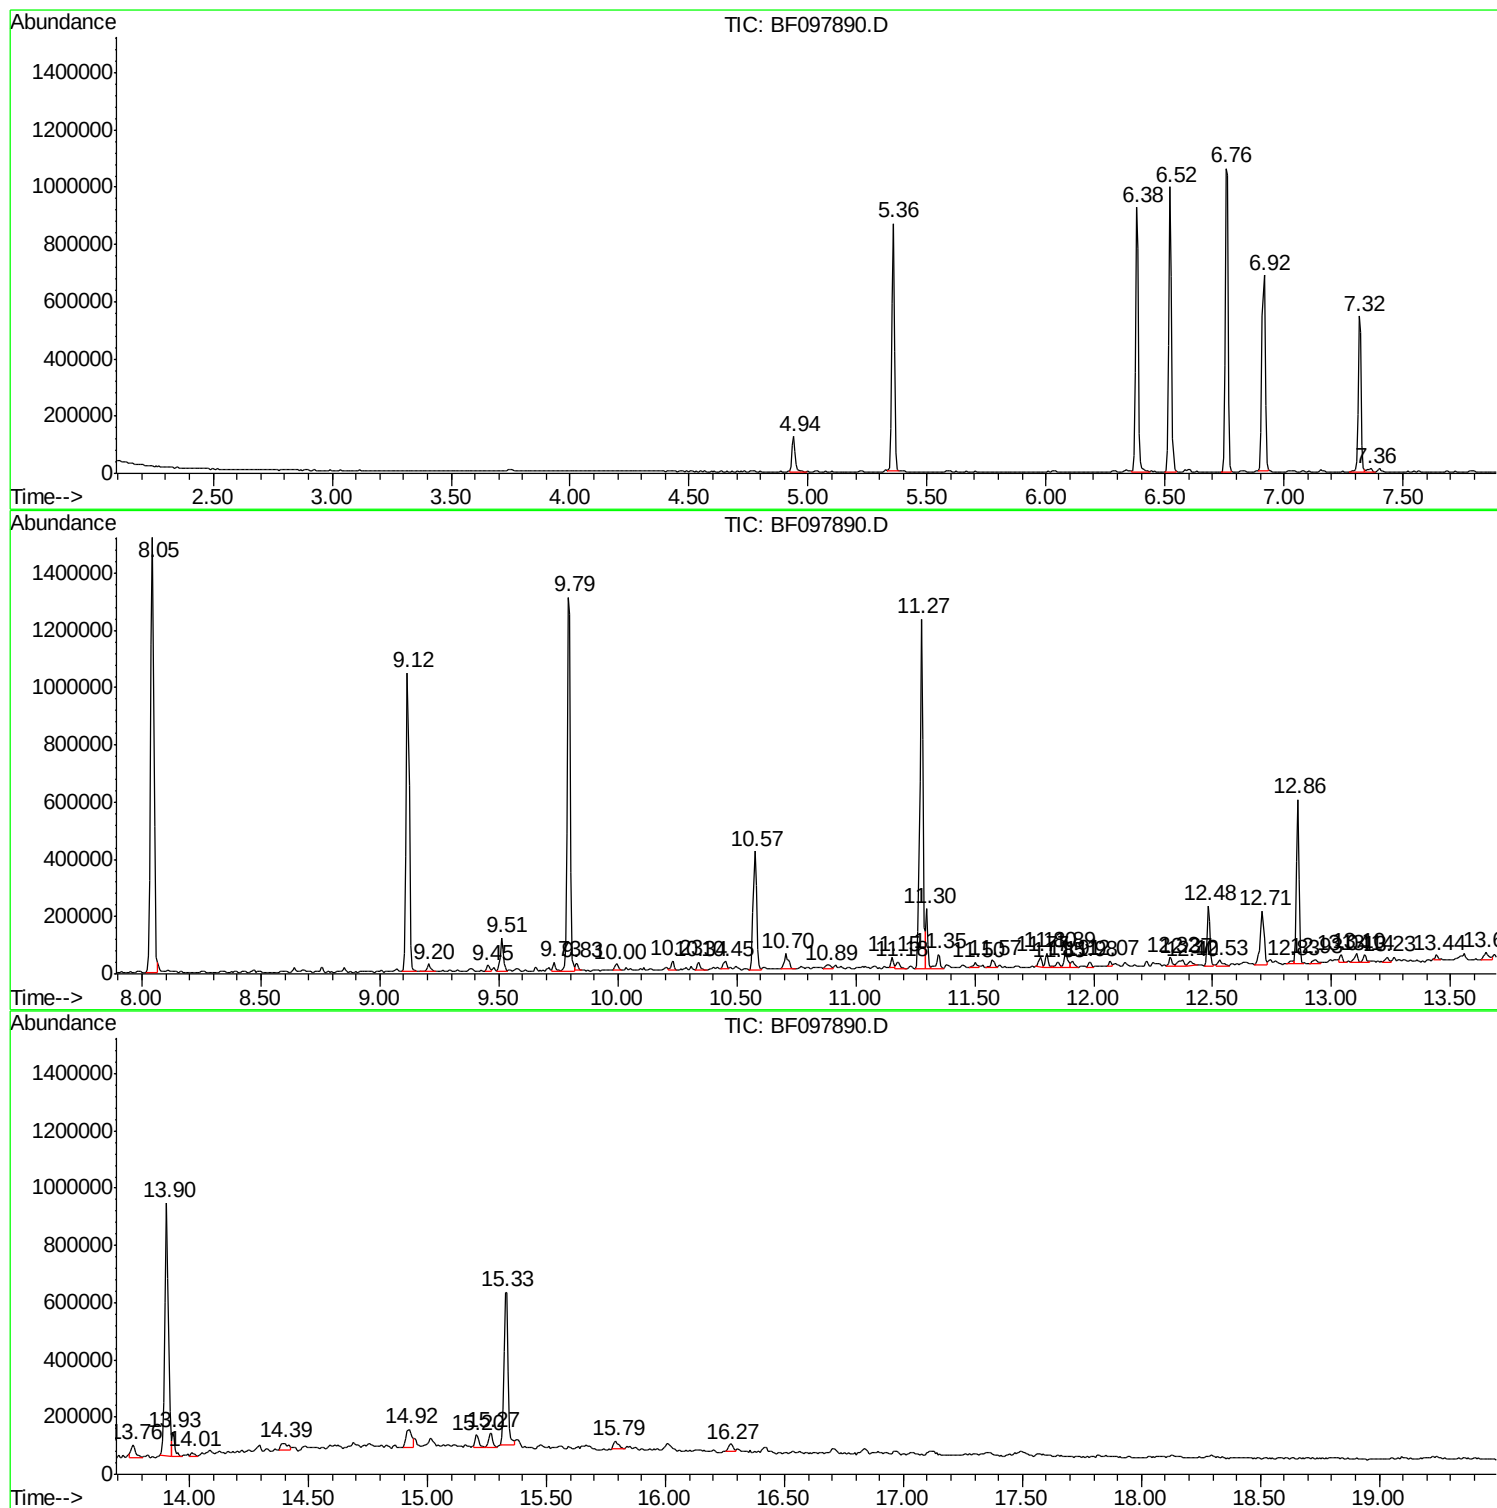

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097890.D
Acq On : 19 Aug 2017 20:32
Operator : SJ/JU
Sample : I4847-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PVSC-A-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.94	2.53 ng	124142	1,4-Dichlorobenzene-d4	6.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3		Acetone	58	C3H6O	000067-64-1	10
4		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

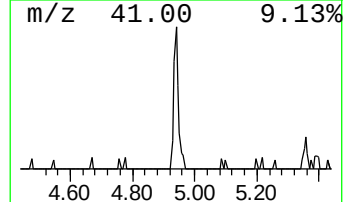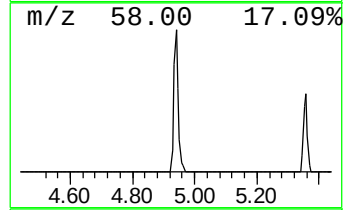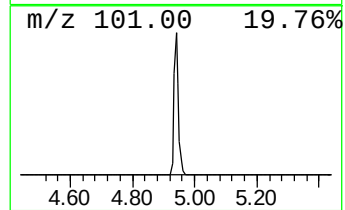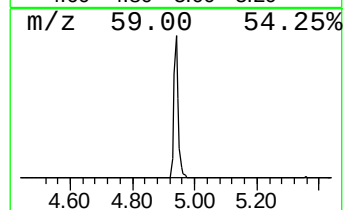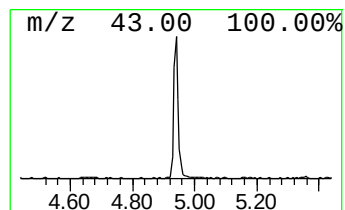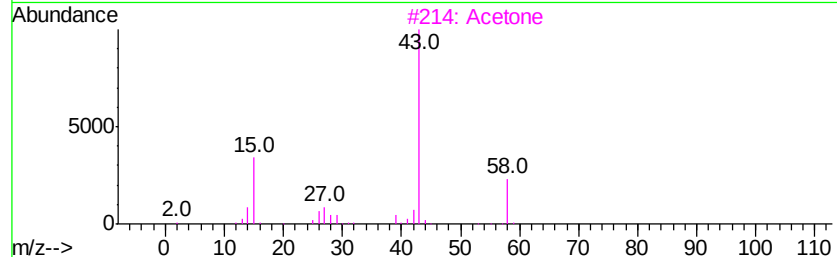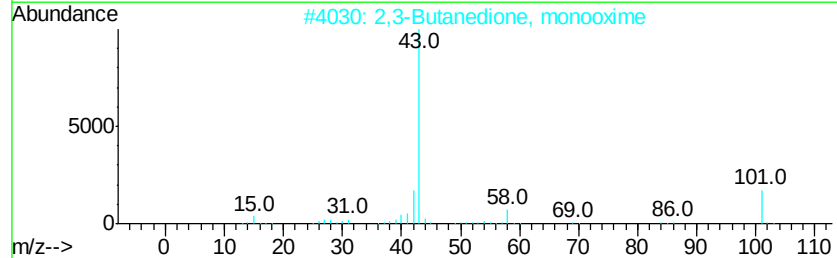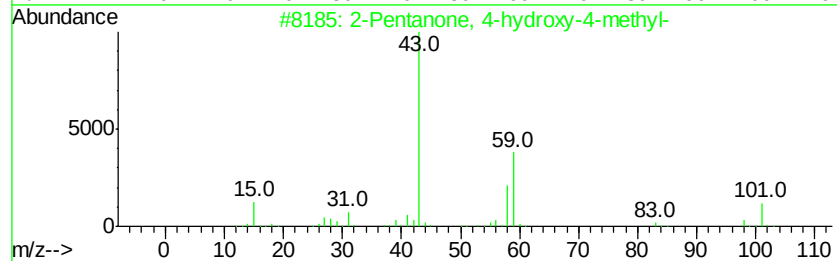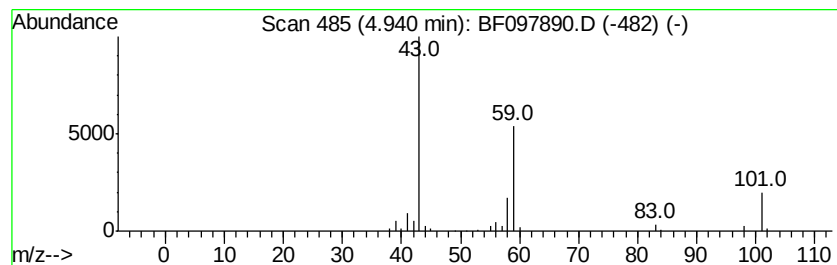

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097890.D
Acq On : 19 Aug 2017 20:32
Operator : SJ/JU
Sample : I4847-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PVSC-A-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	16.68 ng	818608	1,4-Dichlorobenzene-d4	6.76

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	10
4			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

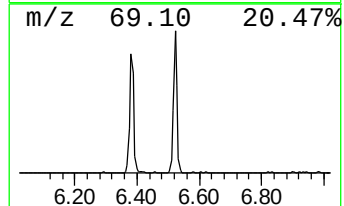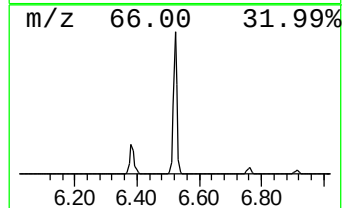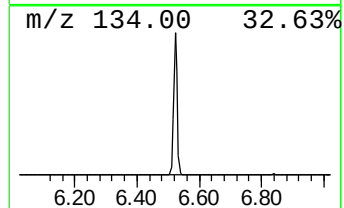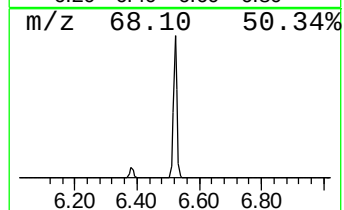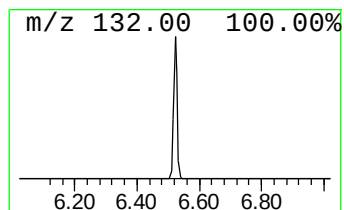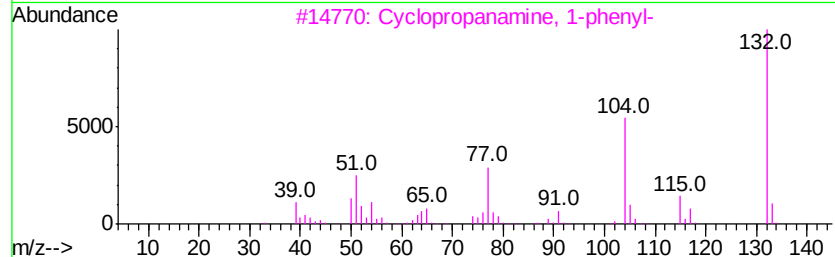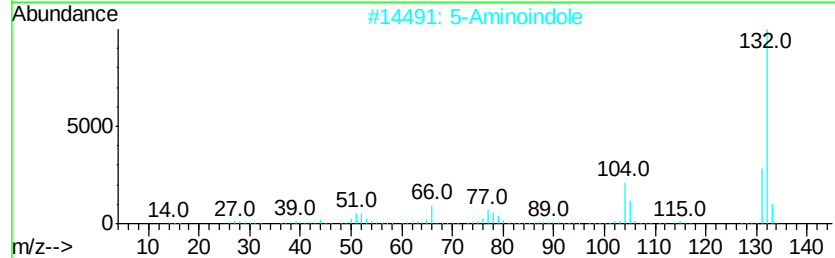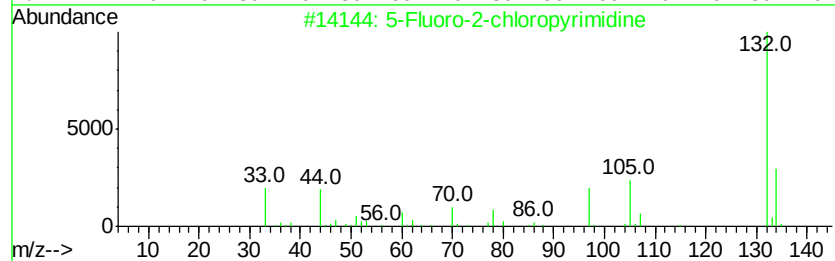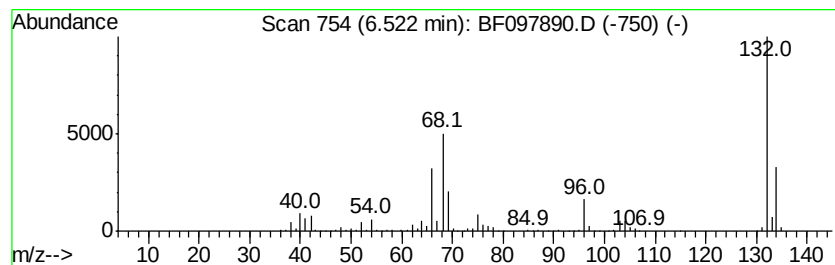

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097890.D
Acq On : 19 Aug 2017 20:32
Operator : SJ/JU
Sample : I4847-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PVSC-A-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.94	2.5	ng	124142	1	6.76	981295	20.0
unknown6.52	6.52	16.7	ng	818608	1	6.76	981295	20.0