

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
 Data File : BF097892.D
 Acq On : 19 Aug 2017 21:28
 Operator : SJ/JU
 Sample : I4852-01 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-207

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.939	482	485	491	rBV	63271	62061	5.23%	0.724%
2	5.357	552	556	563	rVB	469309	403295	34.00%	4.702%
3	6.381	726	730	738	rVB	524749	433999	36.59%	5.060%
4	6.522	751	754	758	rBV	542224	438677	36.98%	5.114%
5	6.763	791	795	798	rBV	1082487	951464	80.22%	11.093%
6	6.916	817	821	824	rBV	384697	311711	26.28%	3.634%
7	7.316	885	889	893	rBV	277231	244866	20.64%	2.855%
8	8.045	1008	1013	1016	rBV	1479428	1186127	100.00%	13.828%
9	9.116	1192	1195	1203	rVB	520345	410085	34.57%	4.781%
10	9.510	1259	1262	1266	rBV	43945	37771	3.18%	0.440%
11	9.798	1307	1311	1314	rBV	1239540	1101921	92.90%	12.847%
12	10.574	1440	1443	1449	rBV	178581	160280	13.51%	1.869%
13	11.274	1558	1562	1565	rBV	1080504	923642	77.87%	10.768%
14	11.298	1565	1566	1569	rVB	46322	27183	2.29%	0.317%
15	12.480	1764	1767	1771	rVB	65796	60455	5.10%	0.705%
16	12.710	1801	1806	1809	rBV	64362	62858	5.30%	0.733%
17	12.857	1828	1831	1835	rBV	307025	244280	20.59%	2.848%
18	13.904	2005	2009	2013	rBV	796332	812219	68.48%	9.469%
19	13.933	2013	2014	2018	rVB	37599	21614	1.82%	0.252%
20	14.921	2179	2182	2185	rBV2	33922	51503	4.34%	0.600%
21	15.333	2247	2252	2258	rBV	481868	590750	49.80%	6.887%
22	15.792	2328	2330	2336	rVB2	30613	40752	3.44%	0.475%


Sum of corrected areas: 8577513

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097892.D
Acq On : 19 Aug 2017 21:28
Operator : SJ/JU
Sample : I4852-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-207

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

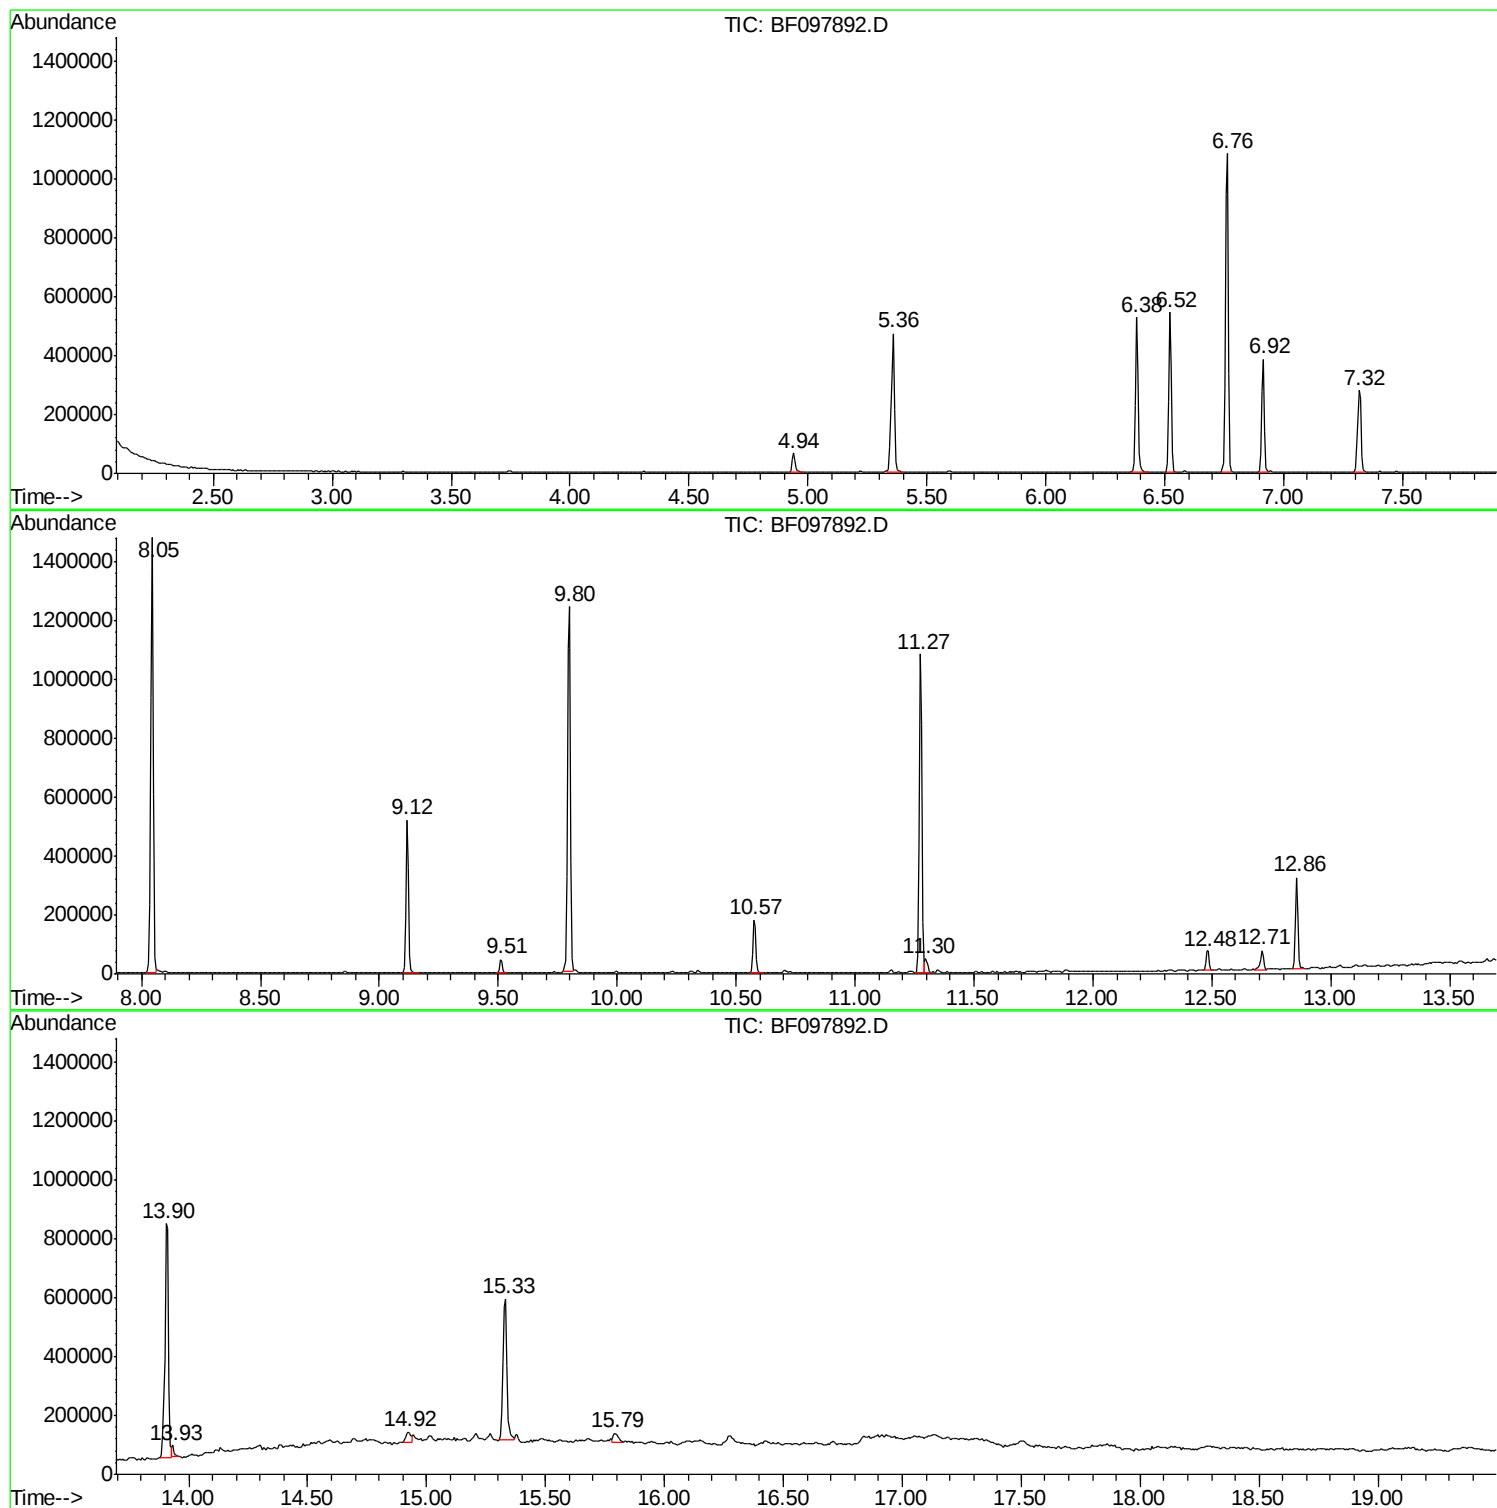

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097892.D
Acq On : 19 Aug 2017 21:28
Operator : SJ/JU
Sample : I4852-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-207










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	9.22 ng	438677	1,4-Dichlorobenzene-d4	6.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	10
4		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

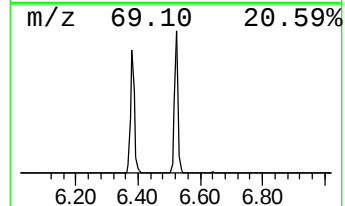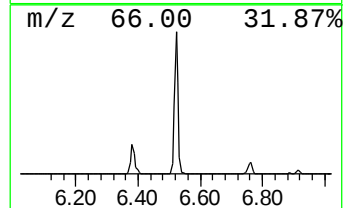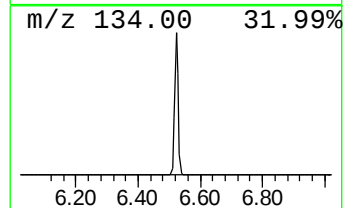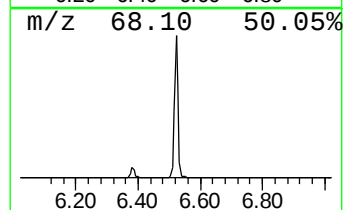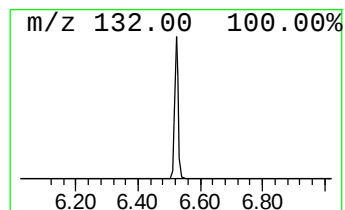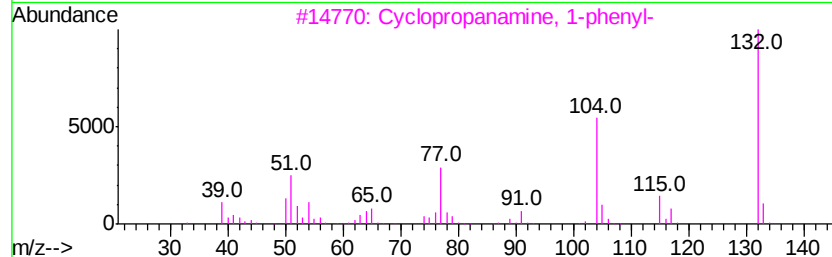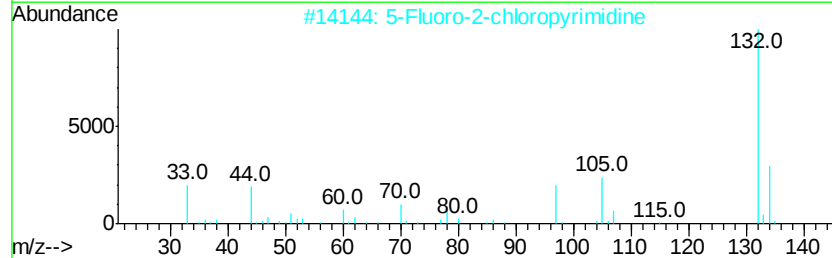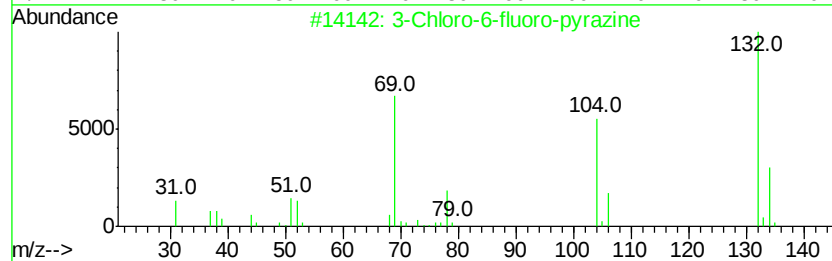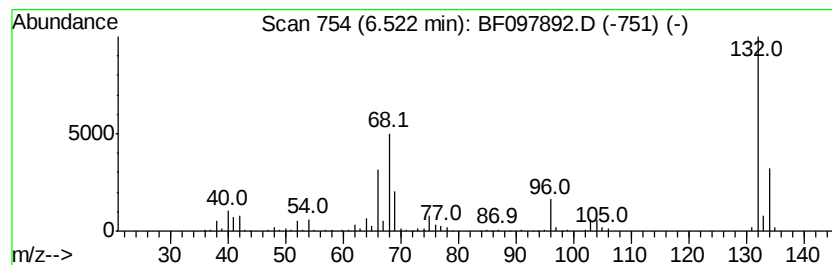

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081917\
Data File : BF097892.D
Acq On : 19 Aug 2017 21:28
Operator : SJ/JU
Sample : I4852-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-207

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	9.2	ng	438677	1	6.76	951464	20.0