


Data Path : Z:\HPCHEM1\BNA F\Data\BF081917\
 Data File : BF097871.D
 Acq On : 19 Aug 2017 11:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

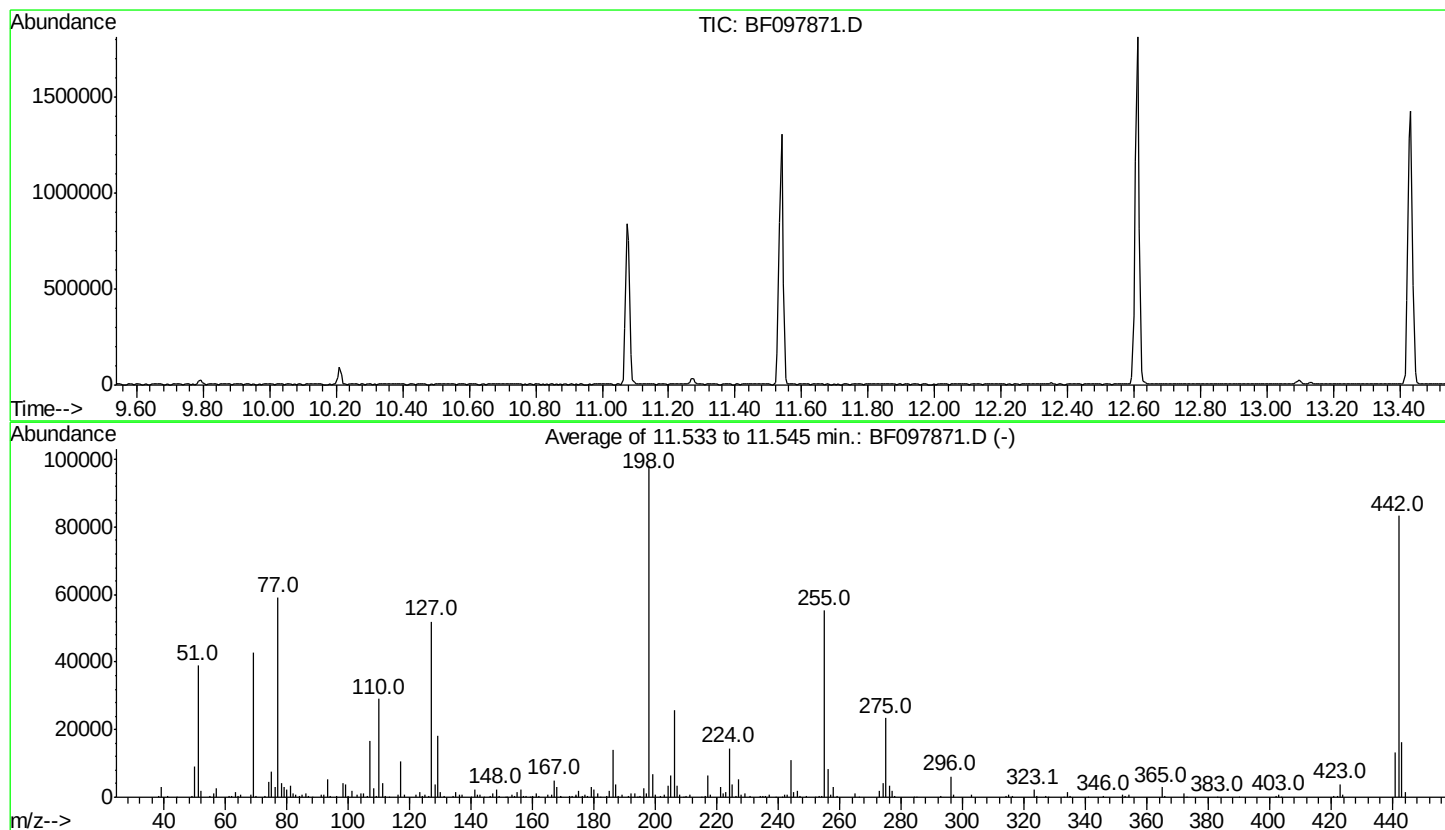

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	38984	PASS
68	69	0.00	2	1.9	827	PASS
69	198	0.00	100	43.7	42891	PASS
70	69	0.00	2	0.6	262	PASS
127	198	10	80	52.9	51960	PASS
197	198	0.00	2	1.0	1002	PASS
198	198	100	100	100.0	98157	PASS
199	198	5	9	6.9	6756	PASS
275	198	10	60	23.8	23317	PASS
365	198	1	100	2.9	2858	PASS
441	442	0.01	24	16.0	13301	PASS
442	198	50	100	84.8	83224	PASS
443	442	15	24	19.7	16433	PASS