
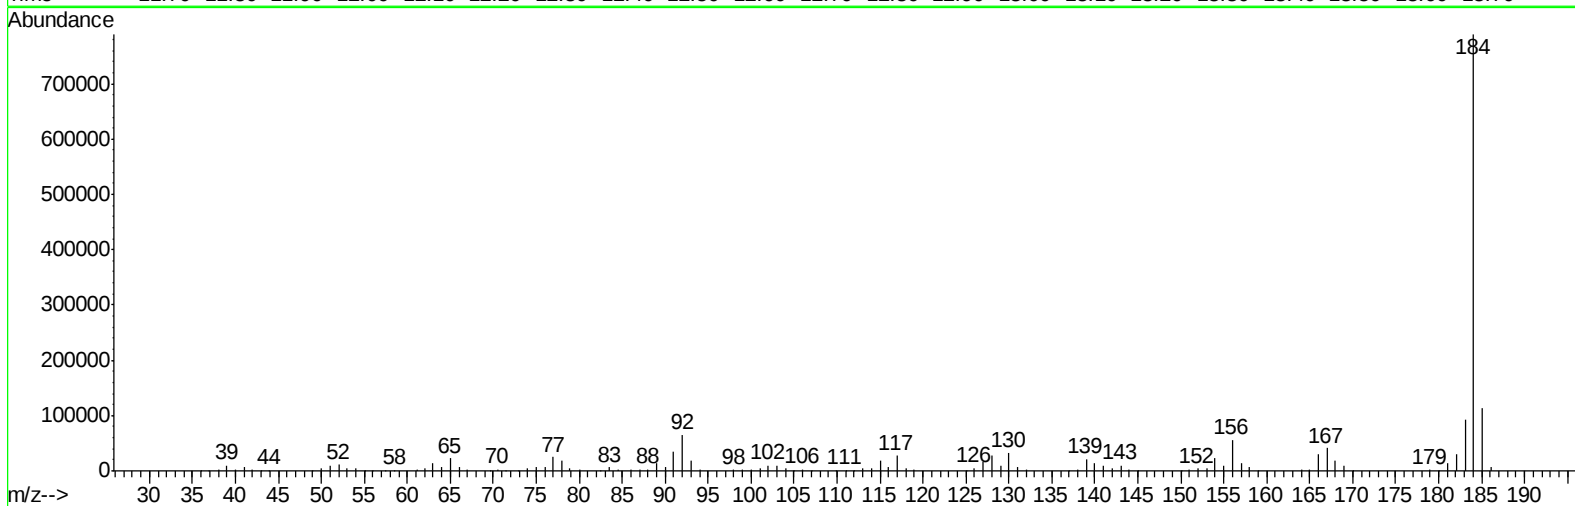


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081919\
 Data File : BF116379.D
 Acq On : 19 Aug 2019 8:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 09:31:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 06:03:31 2019
 Response via : Initial Calibration

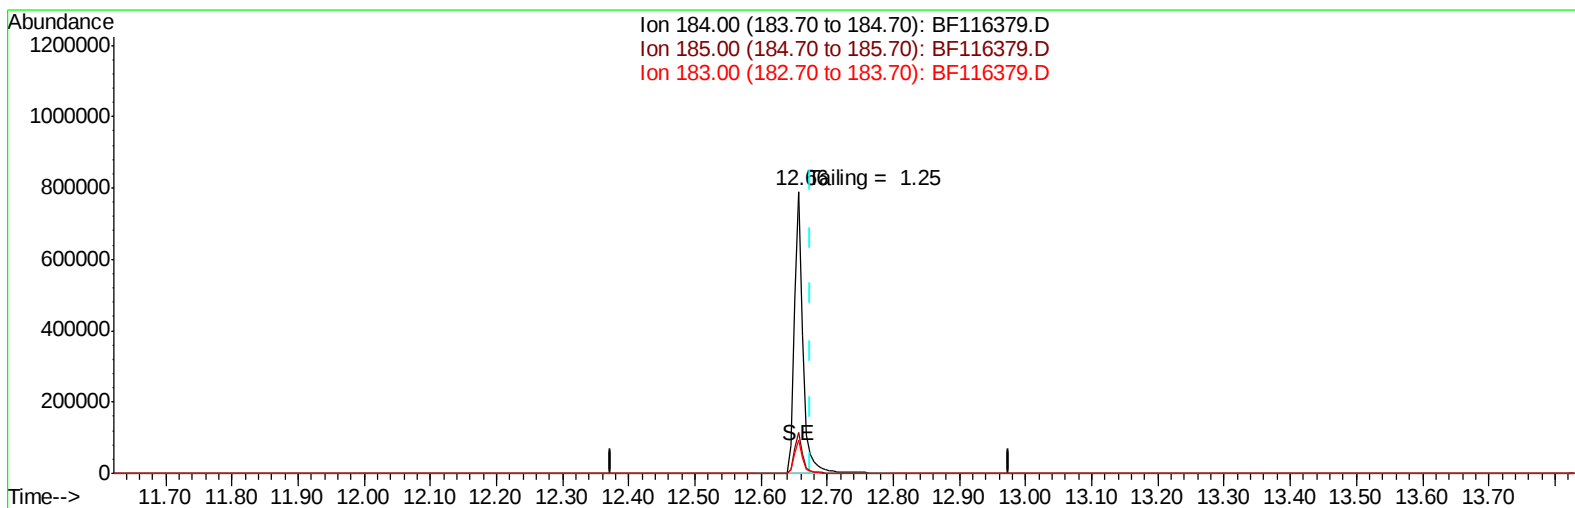

TIC: BF116379.D

(77) Benzidine



12.657min (-0.017) 44821.04ng

response 722294

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.36
183.00	11.70	11.73
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081919\
Data File : BF116379.D
Acq On : 19 Aug 2019 8:30
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 09:31:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 06:03:31 2019
Response via : Initial Calibration

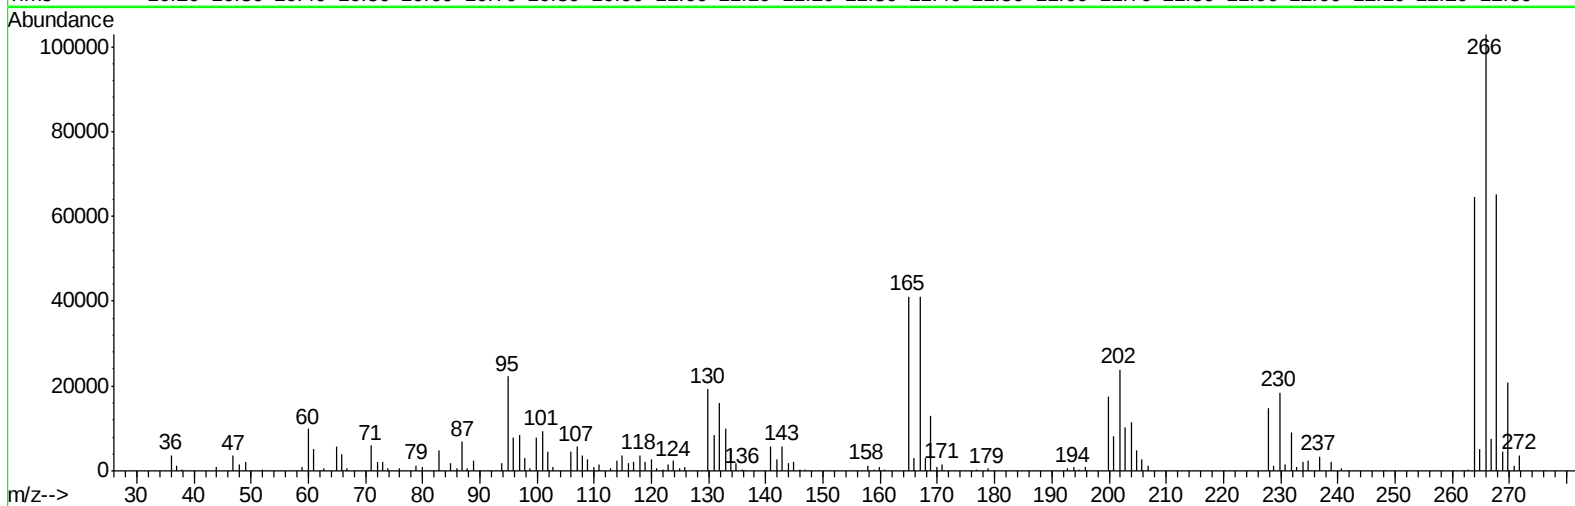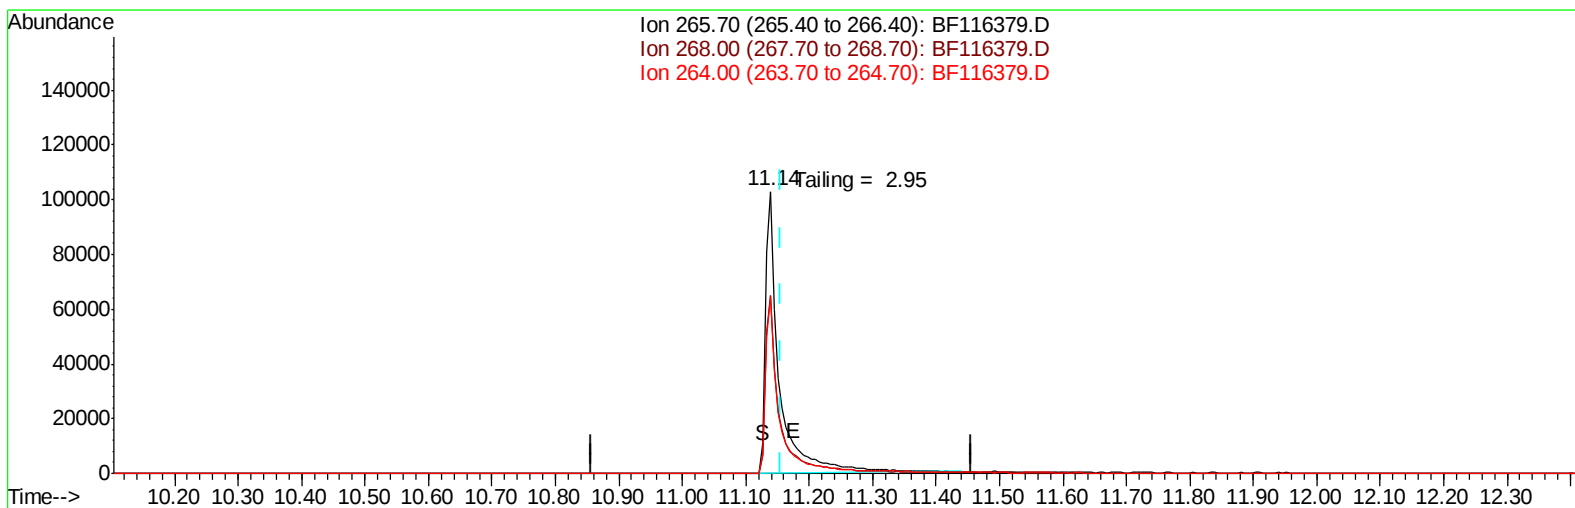

TIC: BF116379.D

(70) Pentachlorophenol (C)

11.139min (-0.017) 23427.15ng

response 159799

Ion	Exp%	Act%
265.70	100	100
268.00	61.00	63.24
264.00	63.30	62.74
0.00	0.00	0.00