
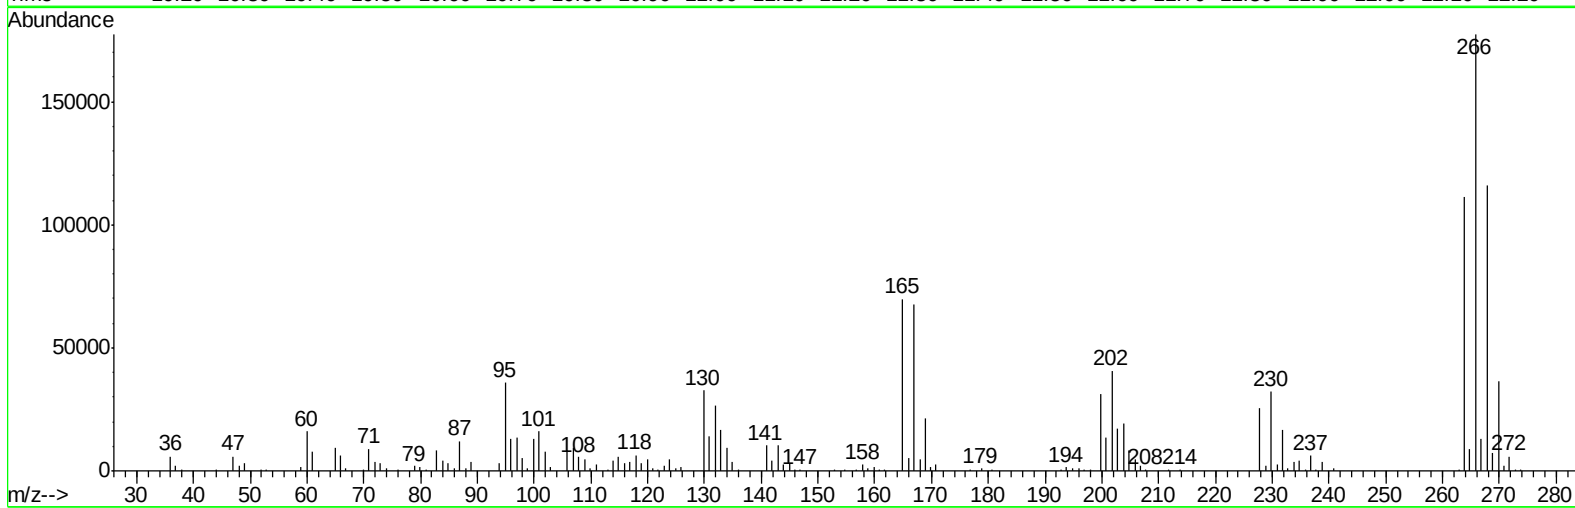


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081919\
Data File : BF116391.D
Acq On : 19 Aug 2019 16:20
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 09:25:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 06:03:31 2019
Response via : Initial Calibration

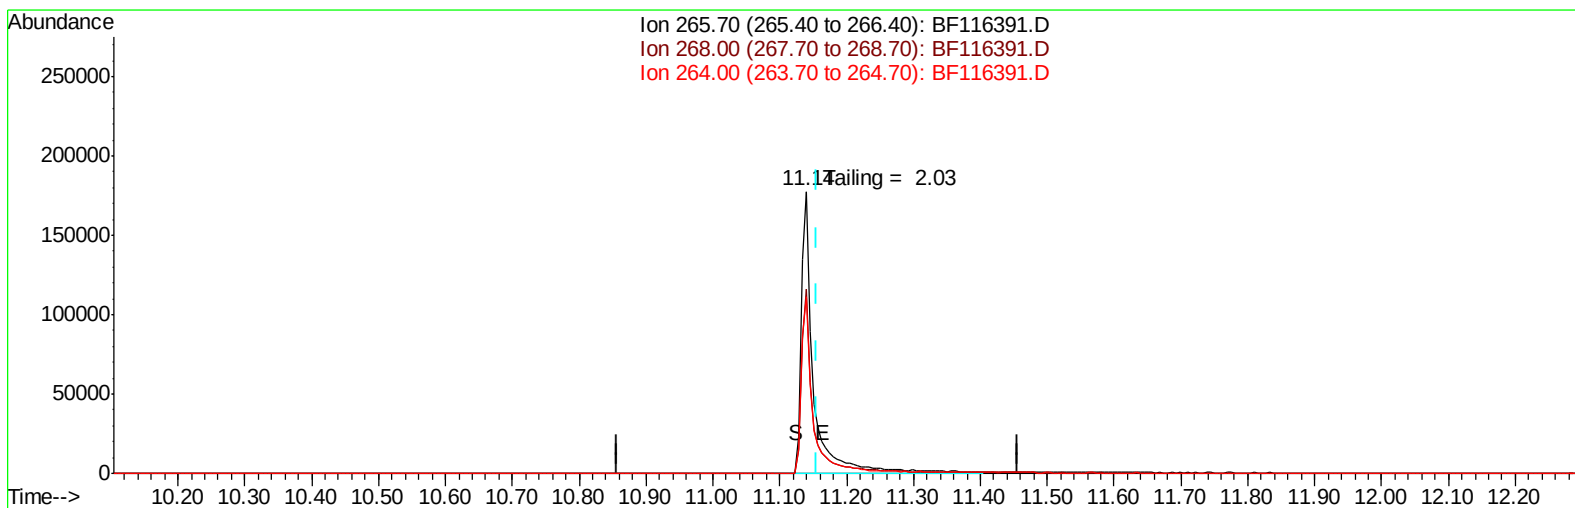

TIC: BF116391.D

(70) Pentachlorophenol (C)



11.139min (-0.017) 24396.56ng

response 224912

Ion	Exp%	Act%
265.70	100	100
268.00	61.00	65.42
264.00	63.30	62.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081919\
Data File : BF116391.D
Acq On : 19 Aug 2019 16:20
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 09:25:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 06:03:31 2019
Response via : Initial Calibration

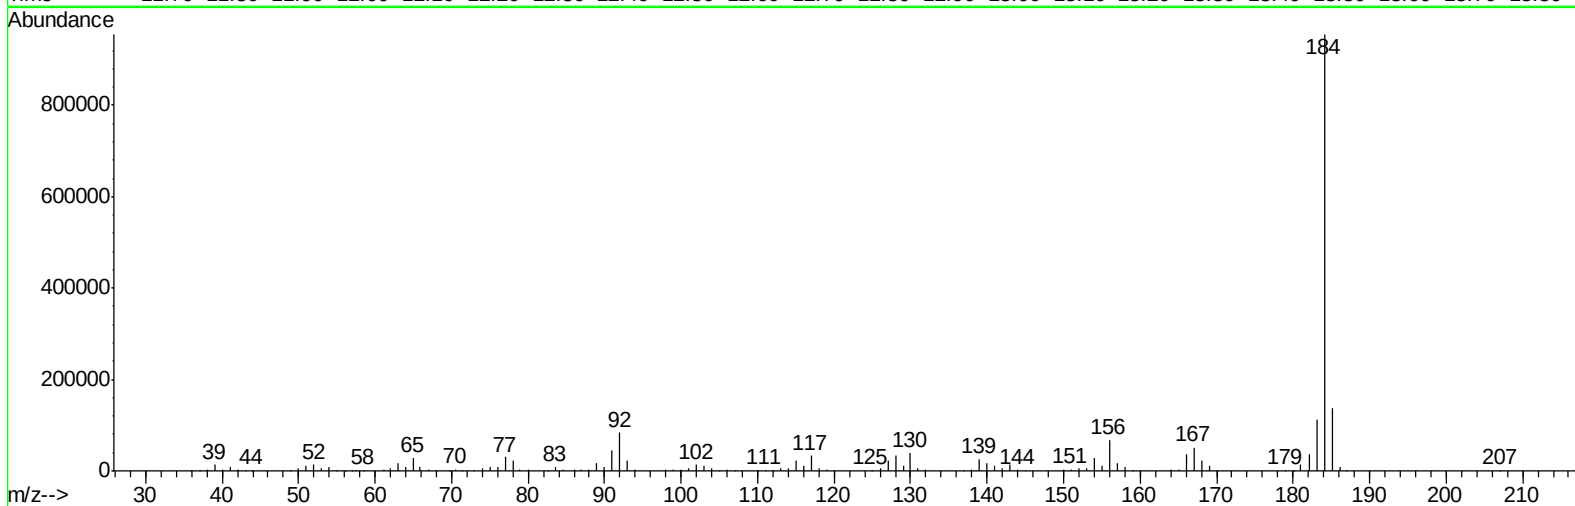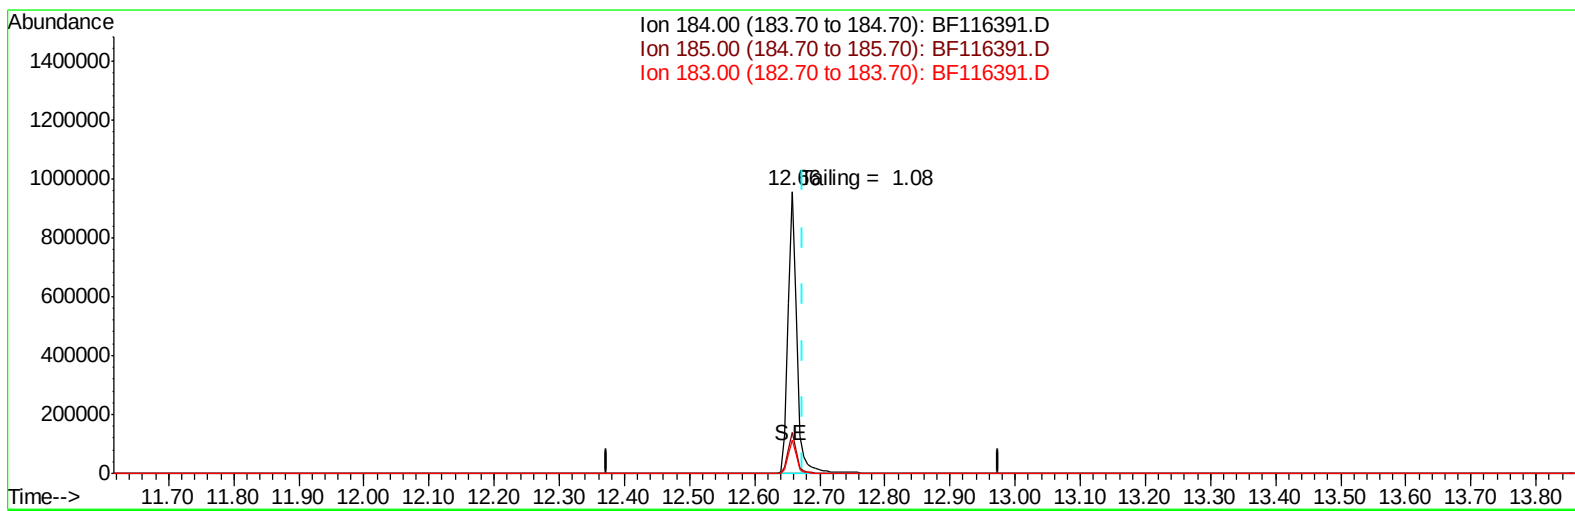

TIC: BF116391.D

(77) Benzidine

12.657min (-0.017) 34586.34ng

response 903229

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.51
183.00	11.70	11.78
0.00	0.00	0.00