

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081919\
 Data File : BF116386.D
 Acq On : 19 Aug 2019 13:36
 Operator : HP/JU
 Sample : K4356-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	3	14	28	rVB	3411698	8423281	100.00%	16.686%
2	2.734	106	110	130	rBV	147715	280799	3.33%	0.556%
3	5.034	497	501	523	rVB	570784	989614	11.75%	1.960%
4	5.445	567	571	601	rBV	2239408	2871136	34.09%	5.688%
5	6.451	738	742	760	rBV	2652346	3005181	35.68%	5.953%
6	6.581	760	764	783	rVB	3666309	3508675	41.65%	6.951%
7	6.804	799	802	813	rVB	997951	884998	10.51%	1.753%
8	6.963	825	829	839	rBV	2982667	3067605	36.42%	6.077%
9	7.369	894	898	921	rBV	2259390	2619583	31.10%	5.189%
10	8.081	1016	1019	1038	rVB	1060215	1139626	13.53%	2.258%
11	9.157	1197	1202	1205	rBV	4342846	4501039	53.44%	8.916%
12	9.551	1266	1269	1280	rBV	699992	594449	7.06%	1.178%
13	9.833	1313	1317	1322	rBV	1507637	1287999	15.29%	2.551%
14	10.627	1448	1452	1467	rBV	2390941	2431161	28.86%	4.816%
15	11.322	1567	1570	1580	rBV	1308767	1183401	14.05%	2.344%
16	12.904	1834	1839	1842	rBV	3845245	3902118	46.33%	7.730%
17	13.786	1984	1989	1991	rBV	146138	155553	1.85%	0.308%
18	13.816	1991	1994	2008	rVB3	71410	186296	2.21%	0.369%
19	13.963	2016	2019	2026	rBV	694846	769193	9.13%	1.524%
20	14.104	2037	2043	2047	rBV	420333	441344	5.24%	0.874%
21	14.410	2089	2095	2099	rBV	897405	956808	11.36%	1.895%
22	14.710	2140	2146	2154	rBV	1297544	1507526	17.90%	2.986%
23	15.033	2195	2201	2212	rBV	1342295	1677970	19.92%	3.324%
24	15.398	2256	2263	2266	rBV	1117074	1625001	19.29%	3.219%
25	15.421	2266	2267	2286	rVB2	504461	641762	7.62%	1.271%
26	15.815	2326	2334	2348	rBV	680252	1141576	13.55%	2.261%
27	16.298	2408	2416	2433	rBV	287506	548322	6.51%	1.086%
28	16.862	2505	2512	2520	rBV	66985	138830	1.65%	0.275%


Sum of corrected areas: 50480846

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081919\
Data File : BF116386.D
Acq On : 19 Aug 2019 13:36
Operator : HP/JU
Sample : K4356-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

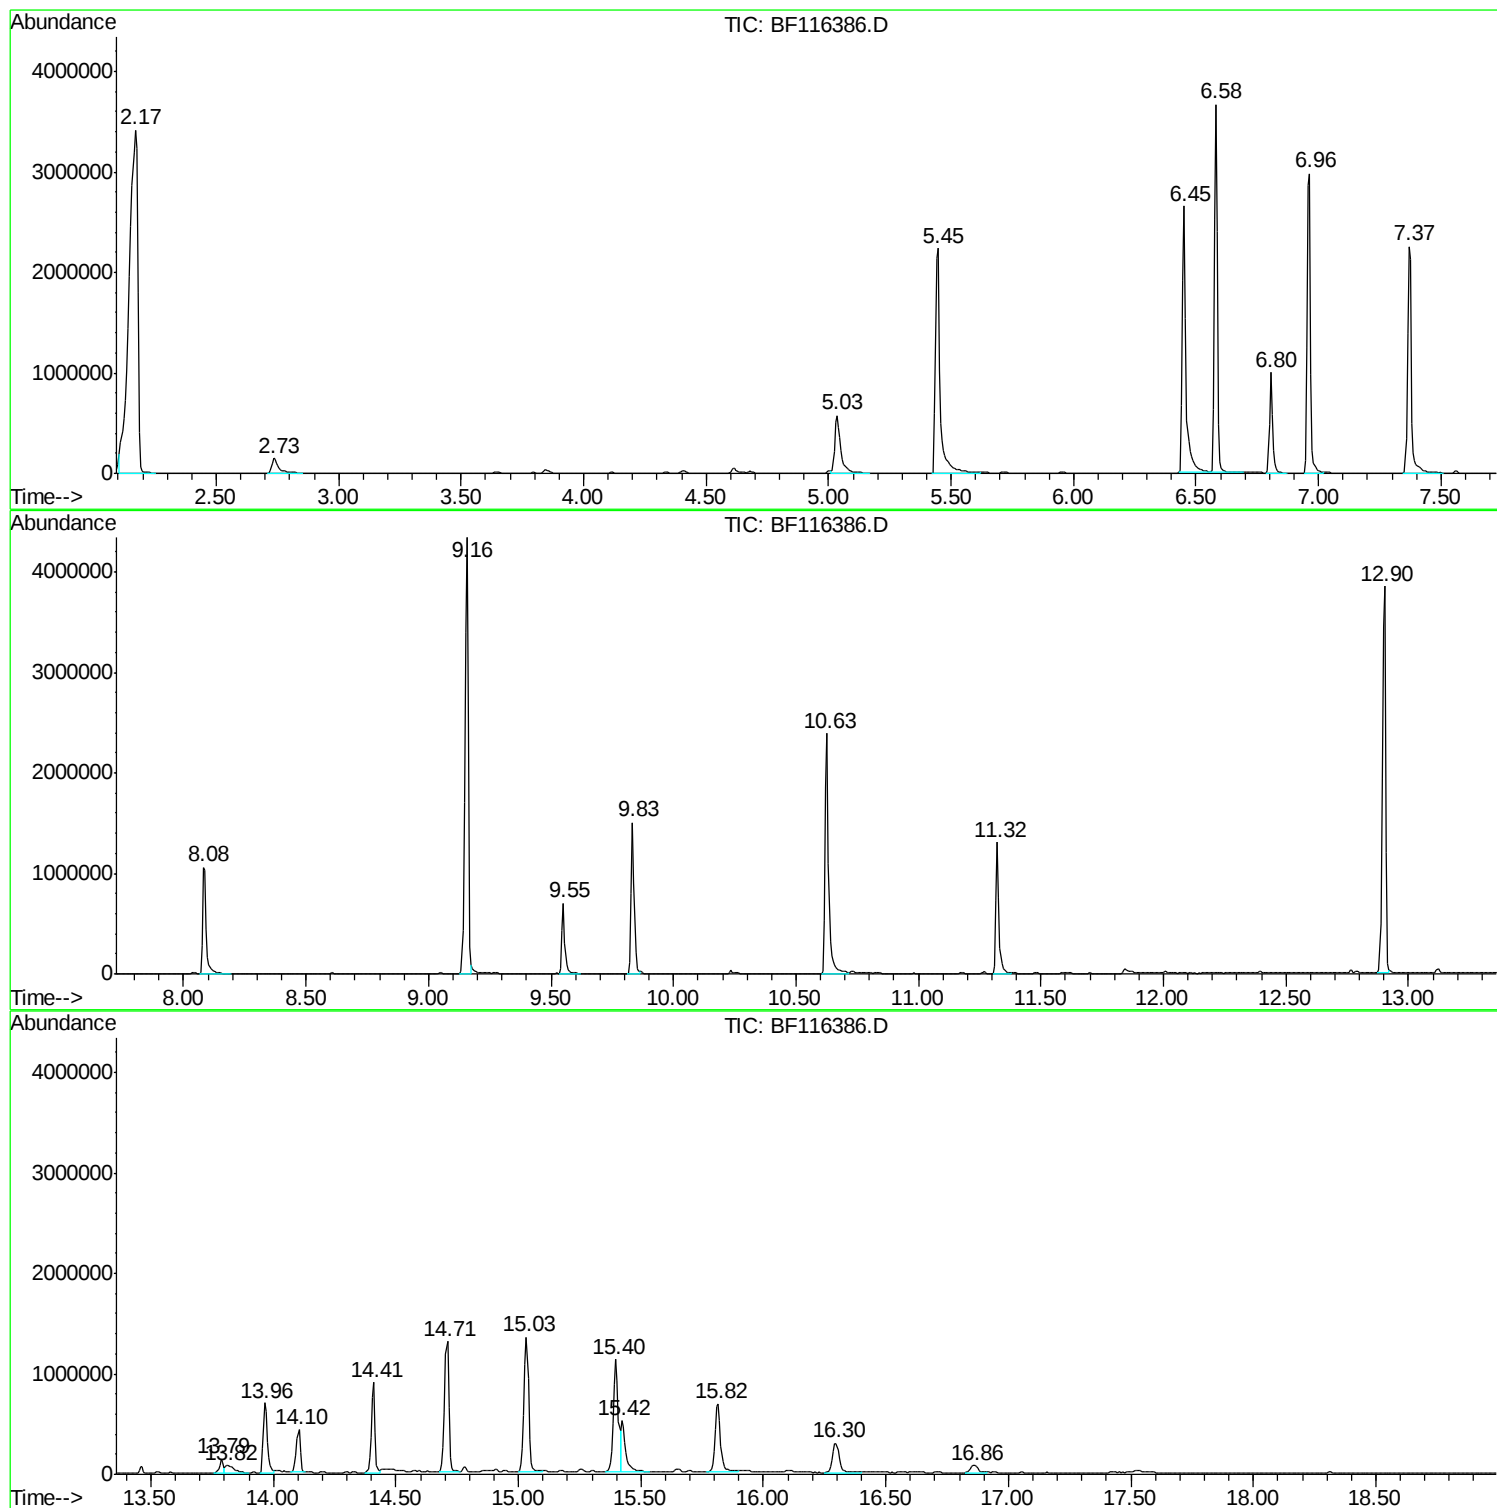

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081919\
Data_File : BF116386.D
Acq_On : 19_Aug_2019_ 13:366
Operator : HP/JUU
Sample : K4356-066
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
TP-3

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
