


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081919\
 Data File : BF116379.D
 Acq On : 19 Aug 2019 8:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

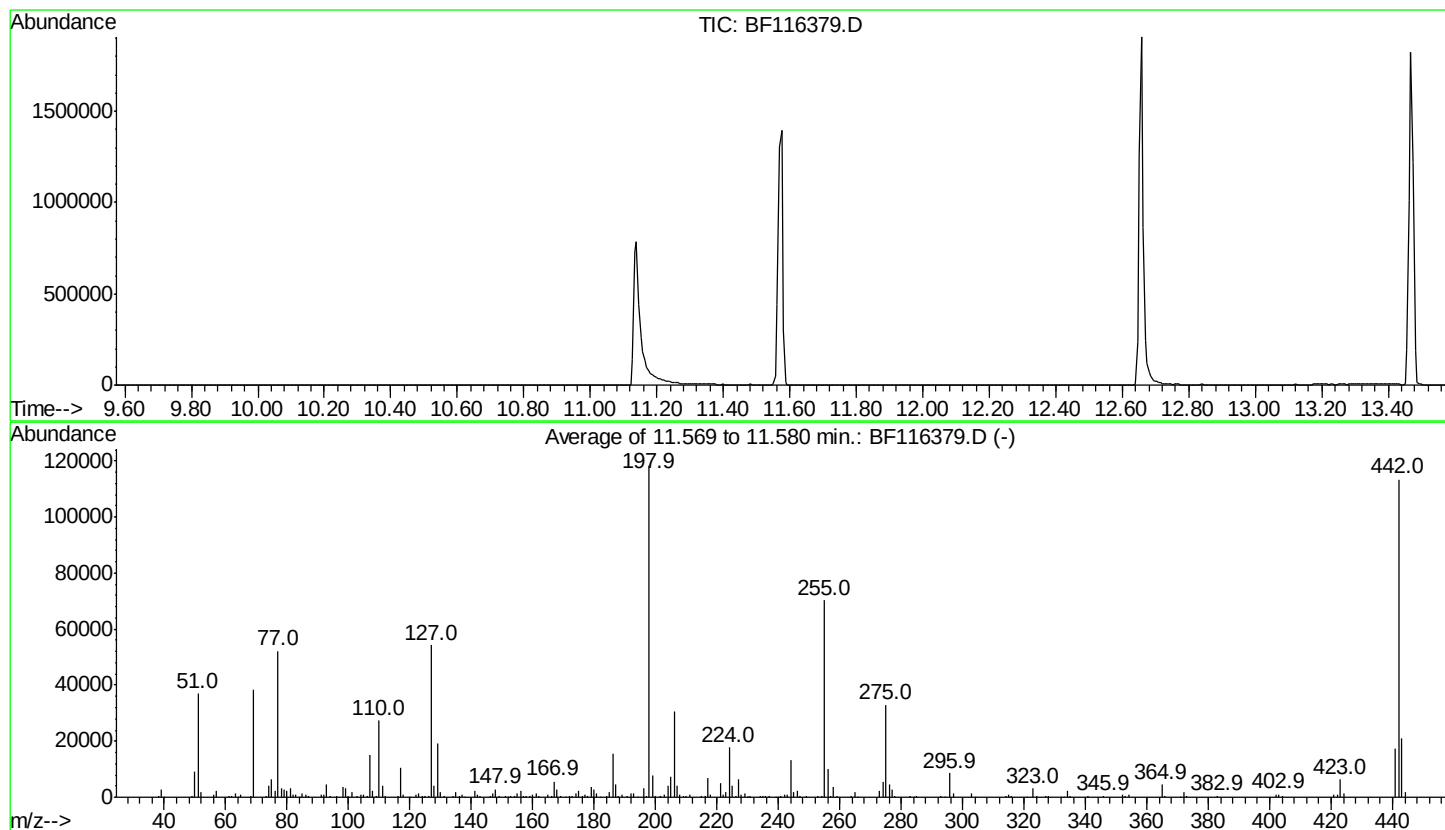

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	36980	PASS
68	69	0.00	2	1.4	547	PASS
69	198	0.00	100	32.3	38211	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	54269	PASS
197	198	0.00	2	0.5	646	PASS
198	198	100	100	100.0	118378	PASS
199	198	5	9	6.4	7599	PASS
275	198	10	60	27.9	32990	PASS
365	198	1	100	3.8	4454	PASS
441	198	0.01	100	14.7	17409	PASS
442	198	50	100	95.9	113501	PASS
443	442	15	24	18.5	20945	PASS