


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081919\
 Data File : BF116415.D
 Acq On : 20 Aug 2019 4:41
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

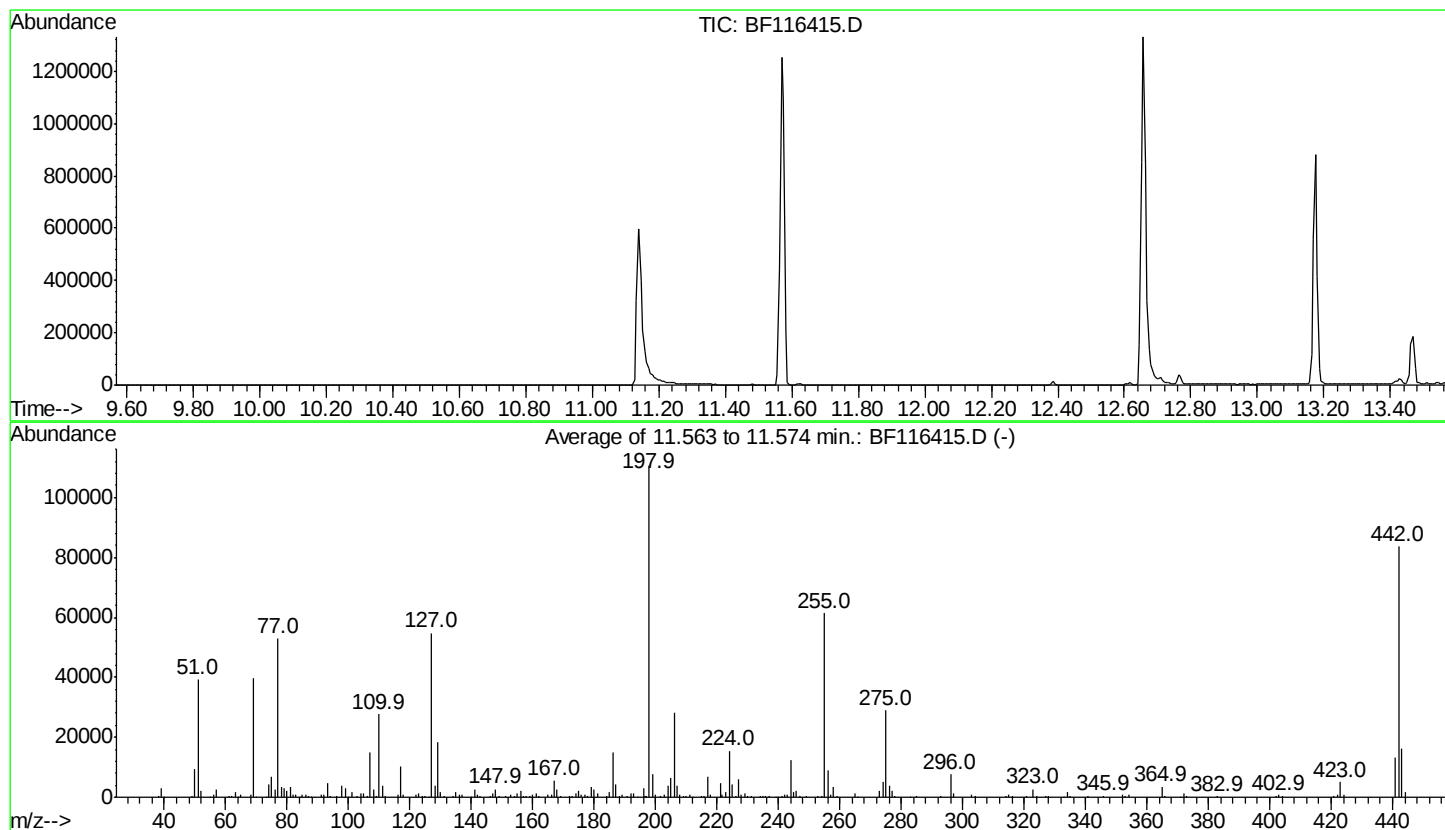

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	39149	PASS
68	69	0.00	2	1.7	694	PASS
69	198	0.00	100	36.1	39888	PASS
70	69	0.00	2	0.3	114	PASS
127	198	10	80	49.4	54680	PASS
197	198	0.00	2	0.3	368	PASS
198	198	100	100	100.0	110618	PASS
199	198	5	9	6.8	7501	PASS
275	198	10	60	26.1	28911	PASS
365	198	1	100	3.1	3459	PASS
441	198	0.01	100	12.1	13416	PASS
442	198	50	100	75.5	83521	PASS
443	442	15	24	19.5	16310	PASS