



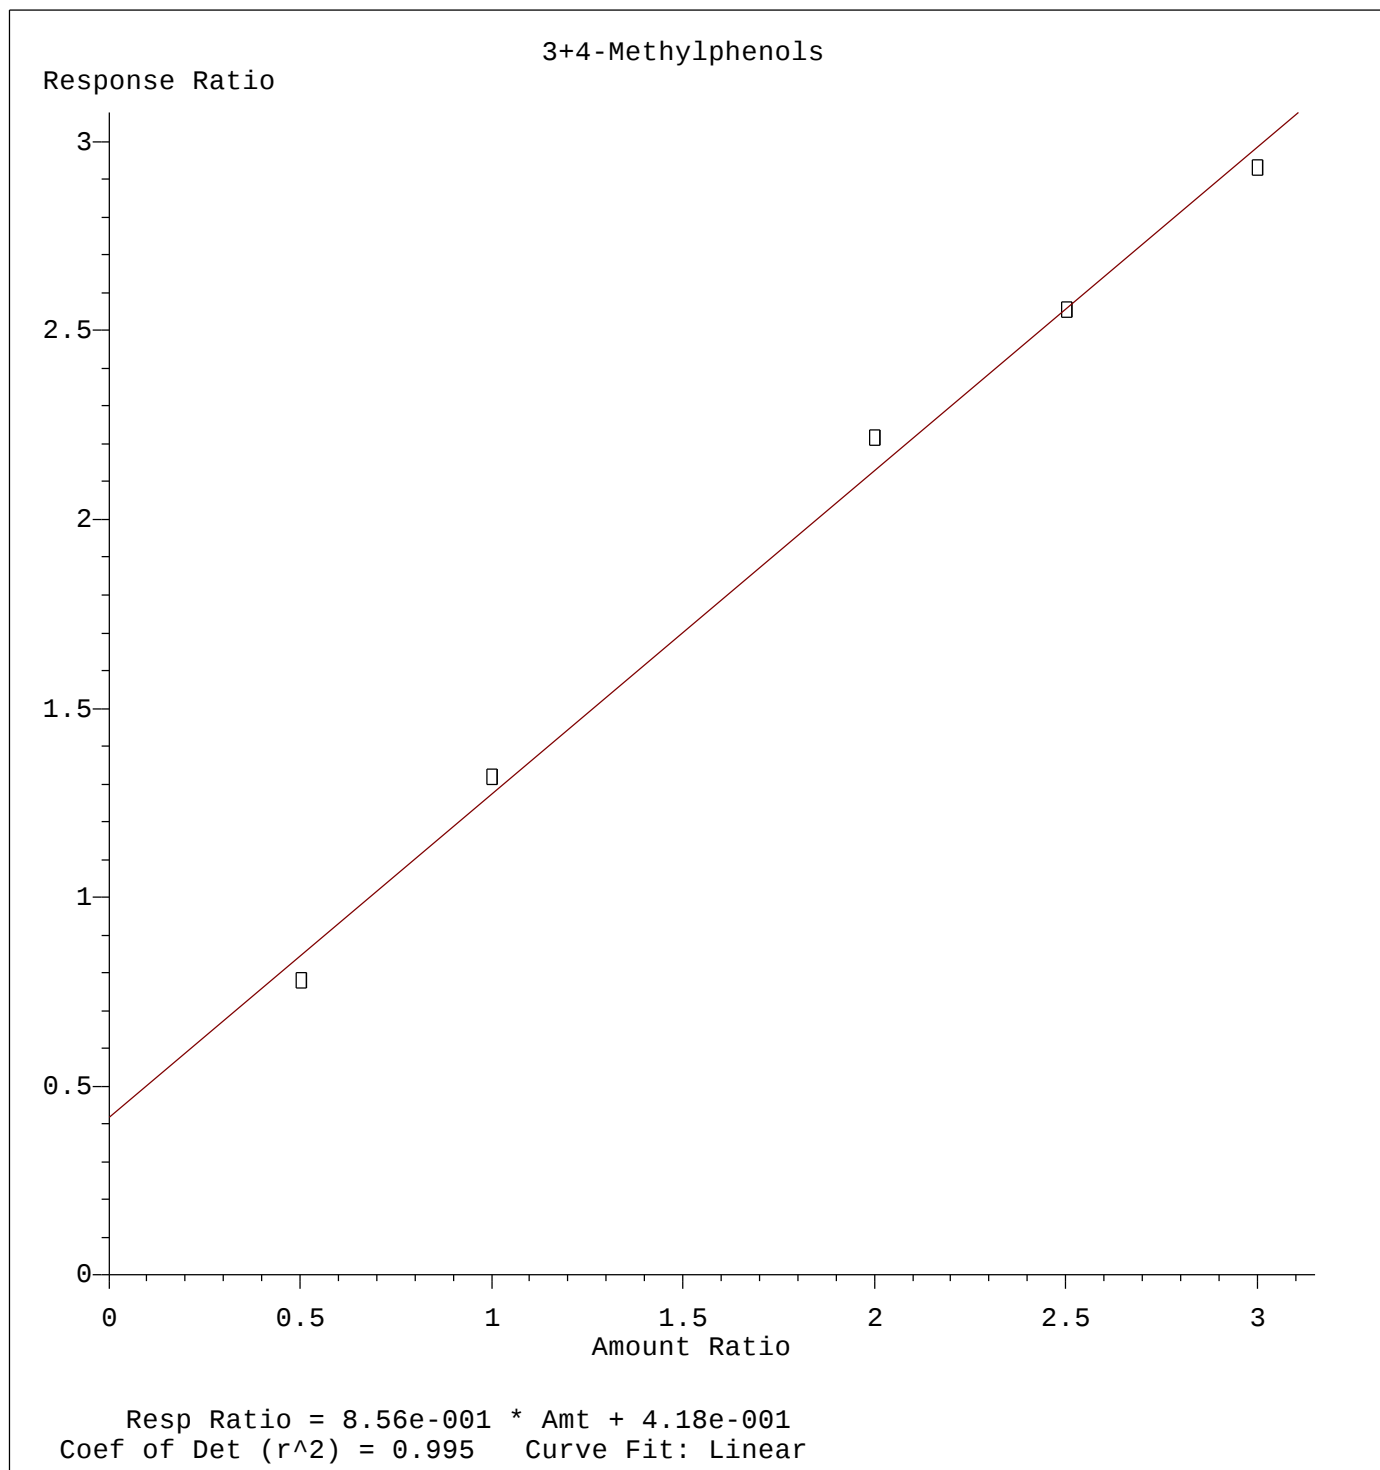


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020

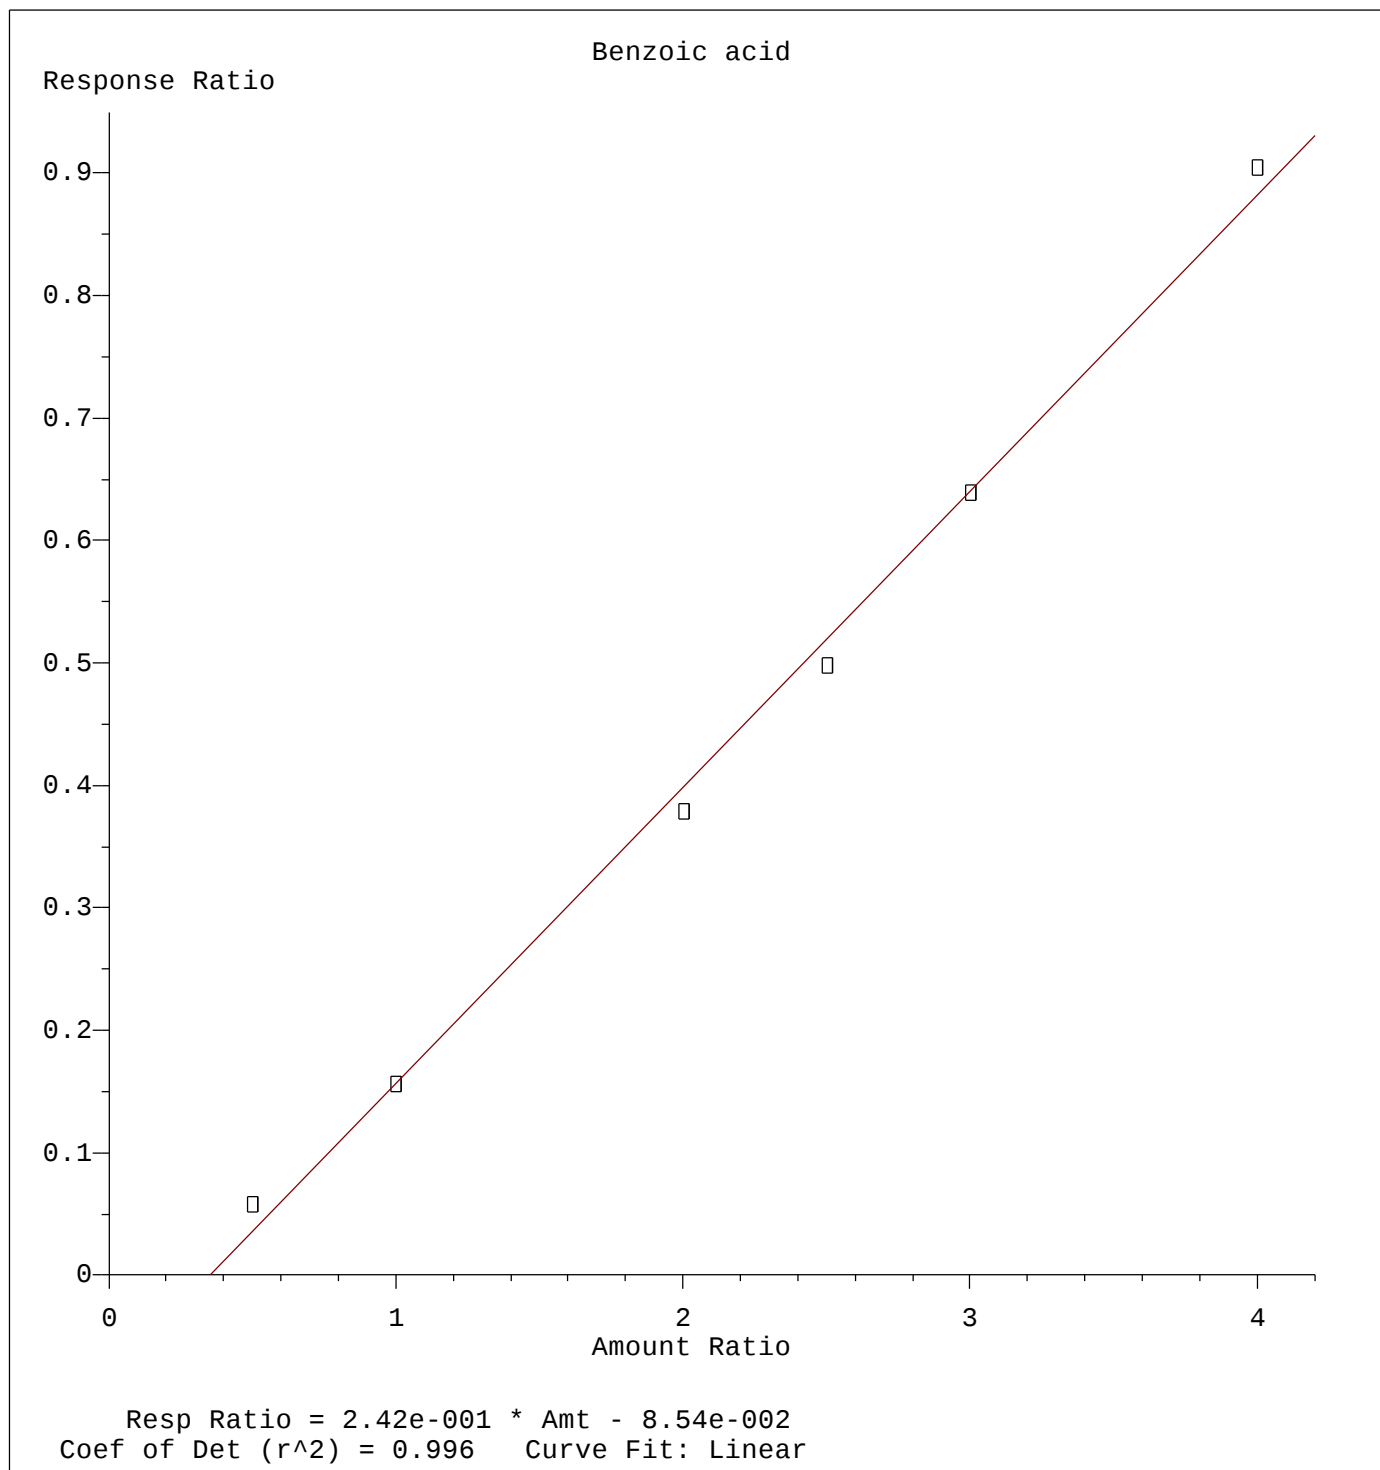

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020


Hexachlorocyclopentadiene

Response Ratio

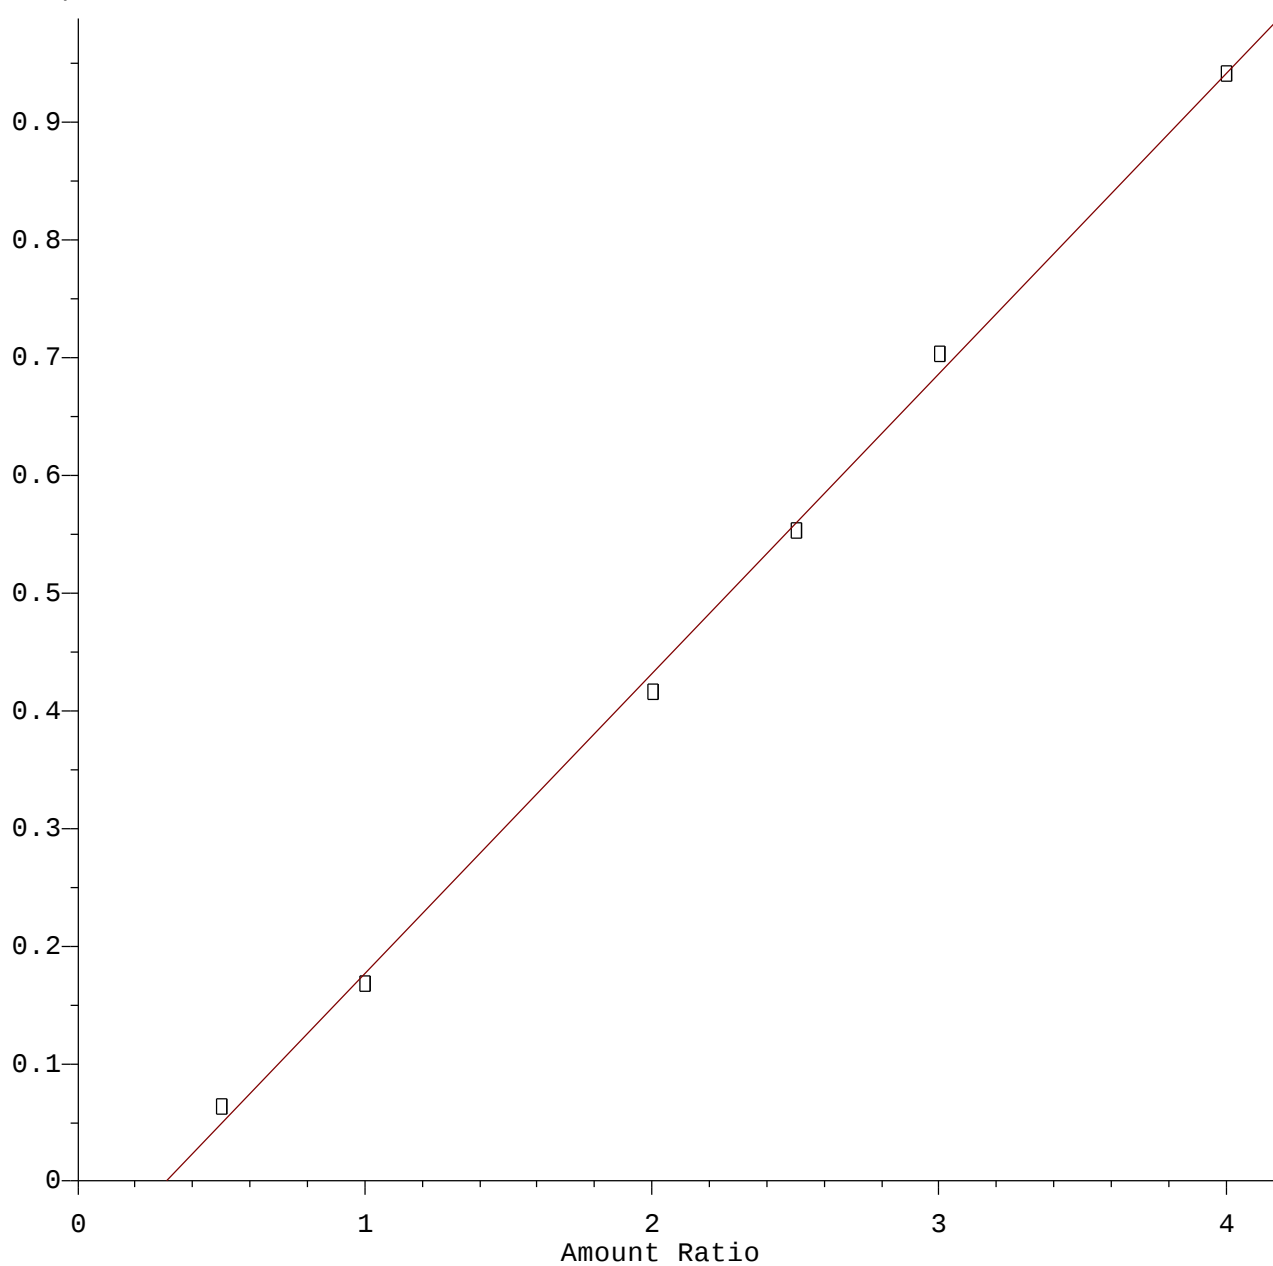

Resp Ratio = $2.55 \times 10^{-1} \times \text{Amt} - 7.87 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020

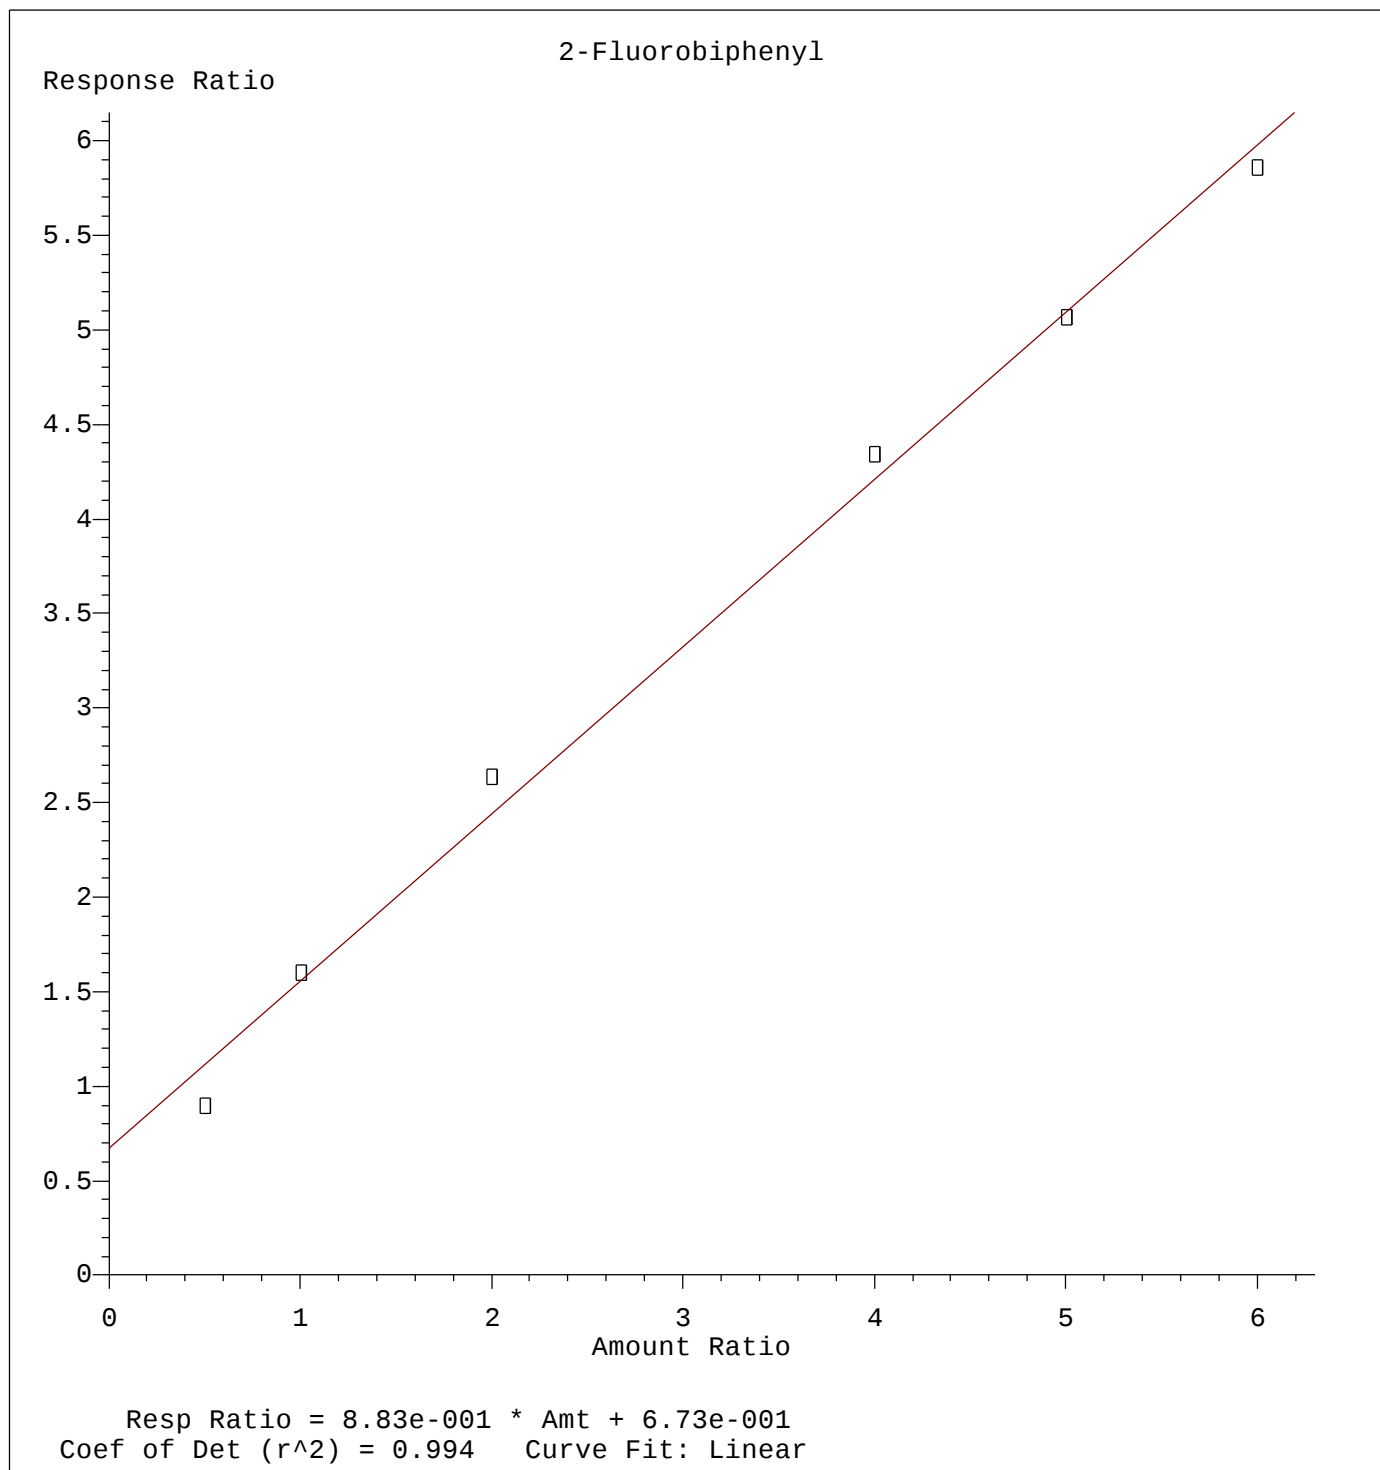

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020


Dibenzofuran

Response Ratio

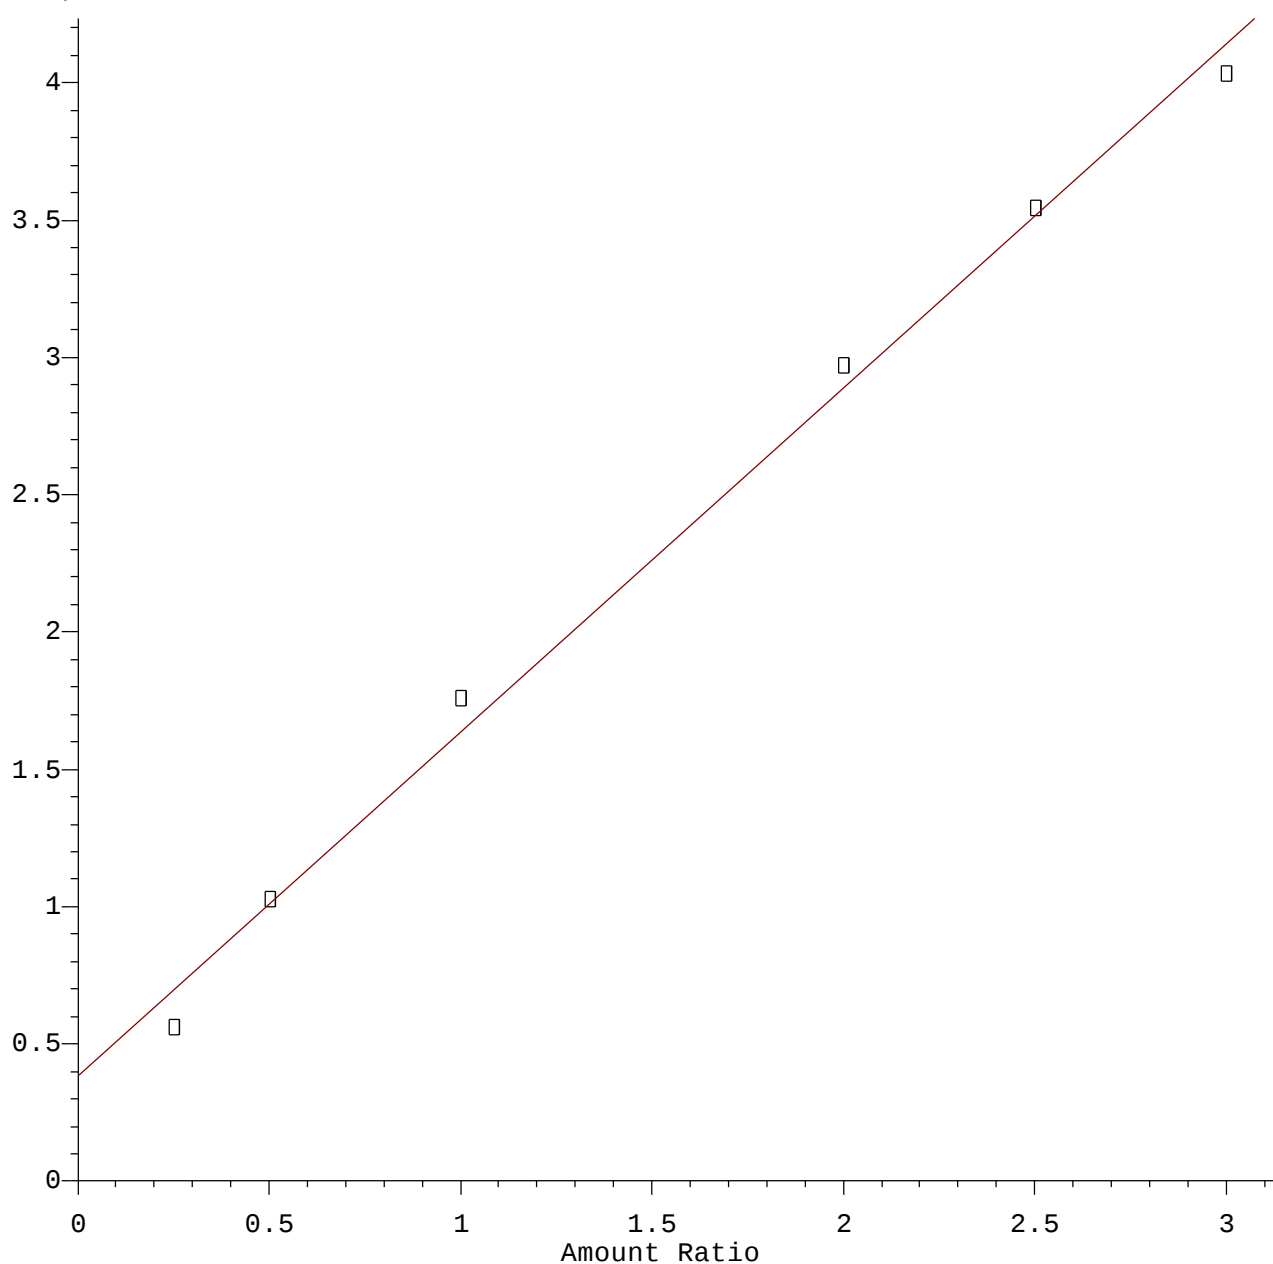

Resp Ratio = 1.25e+000 * Amt + 3.84e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020

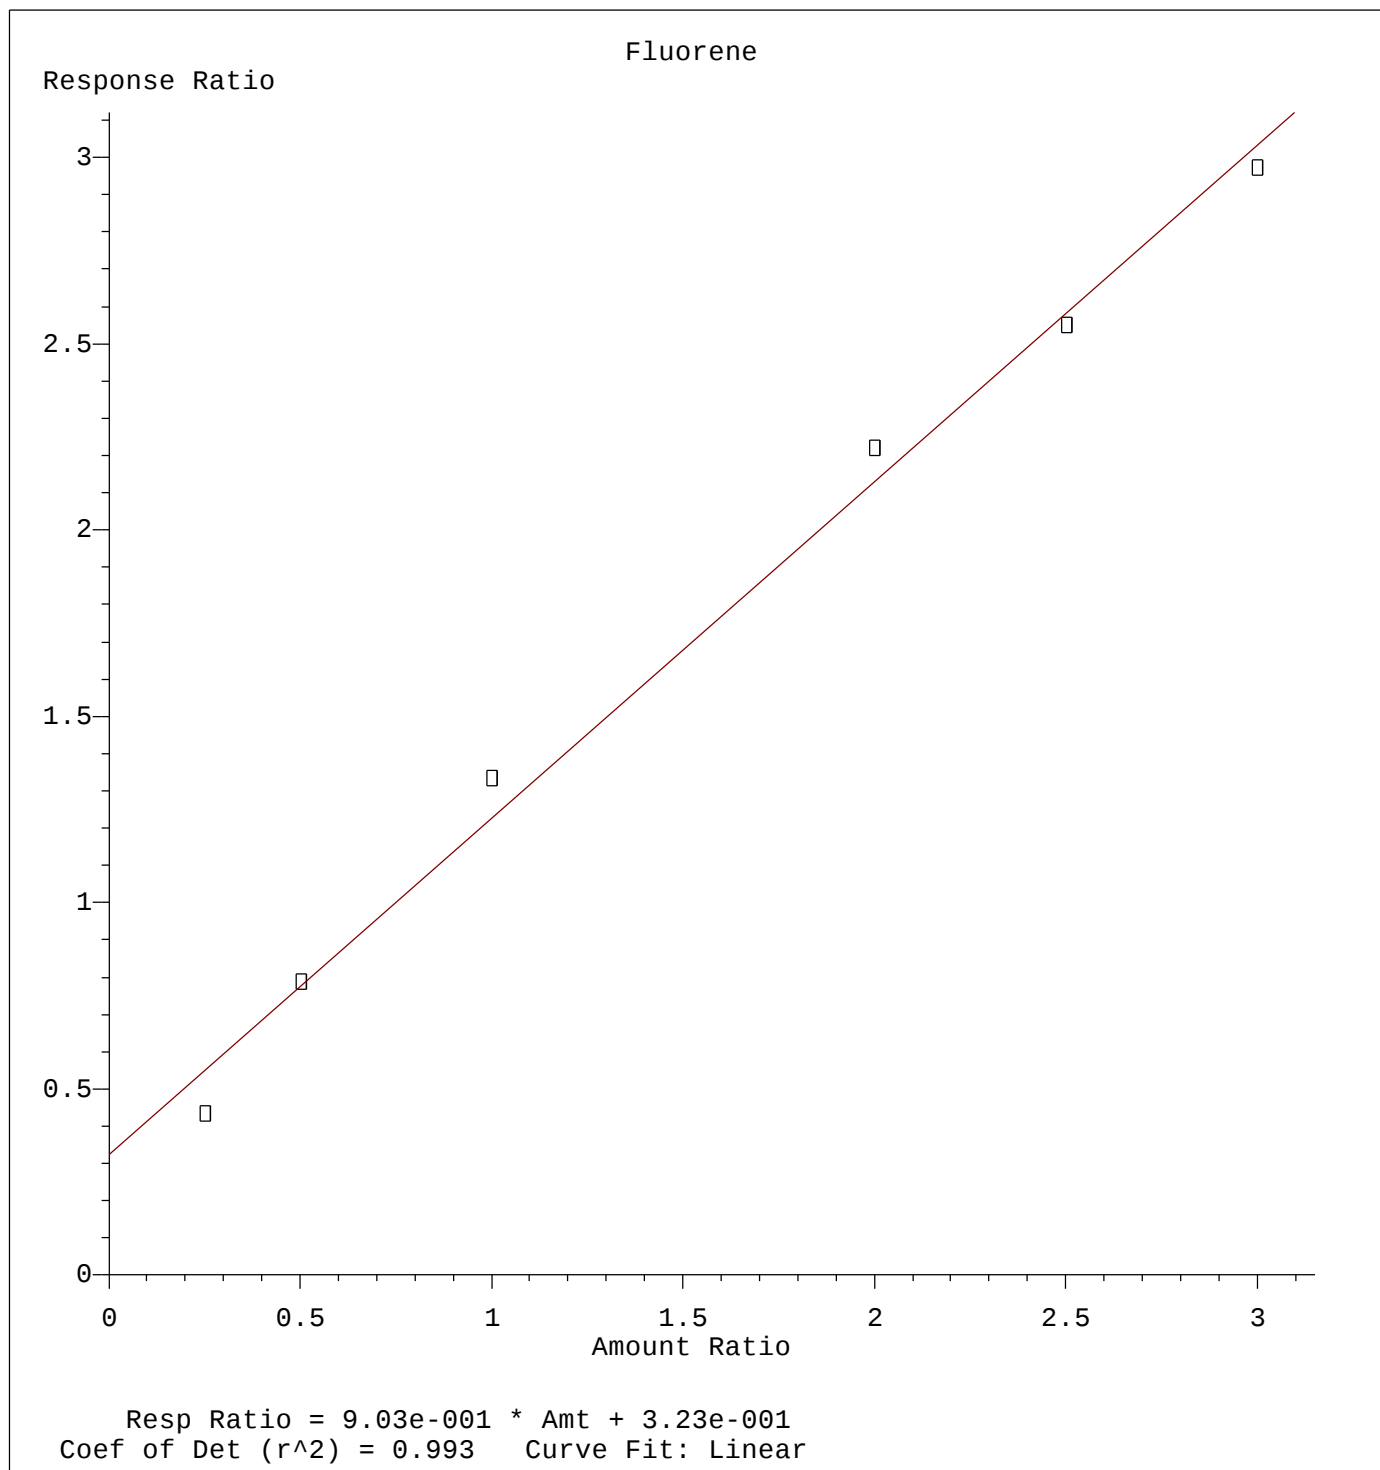

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020

4-Chlorophenyl-phenylether

Response Ratio

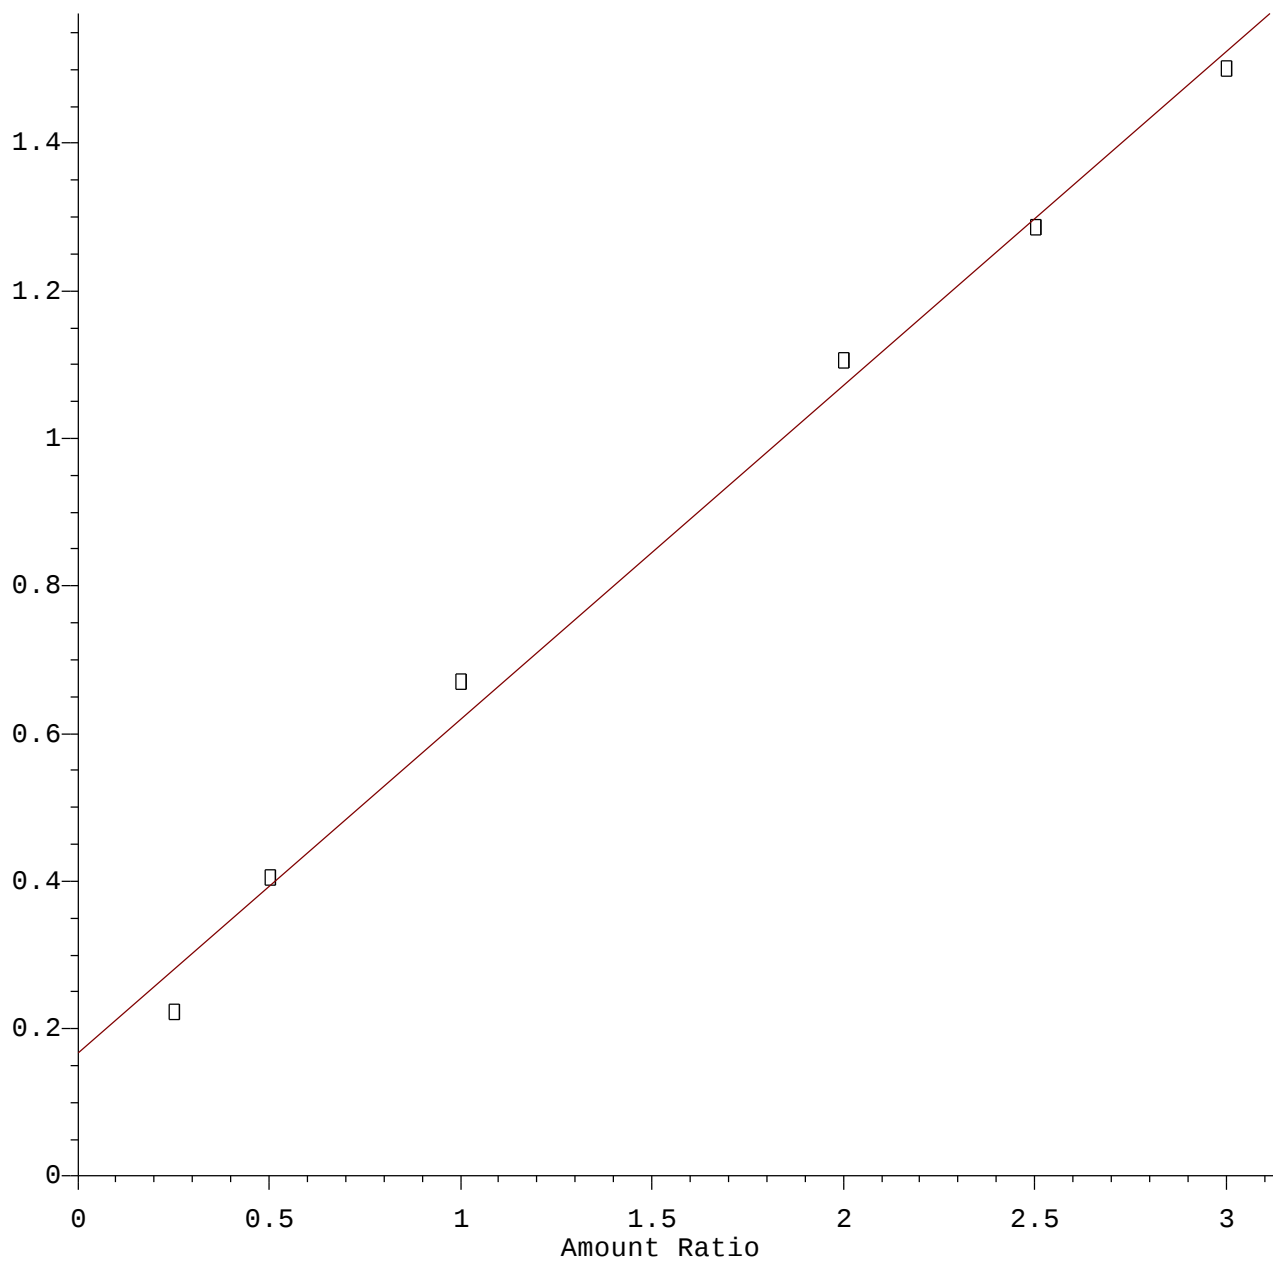

Resp Ratio = $4.53 \times 10^{-1} \times \text{Amt} + 1.66 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
Calibration Table Last Updated: Thu Aug 20 04:56:10 2020