


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081920\
 Data File : BF121324.D
 Acq On : 19 Aug 2020 17:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 20 04:56:10 2020

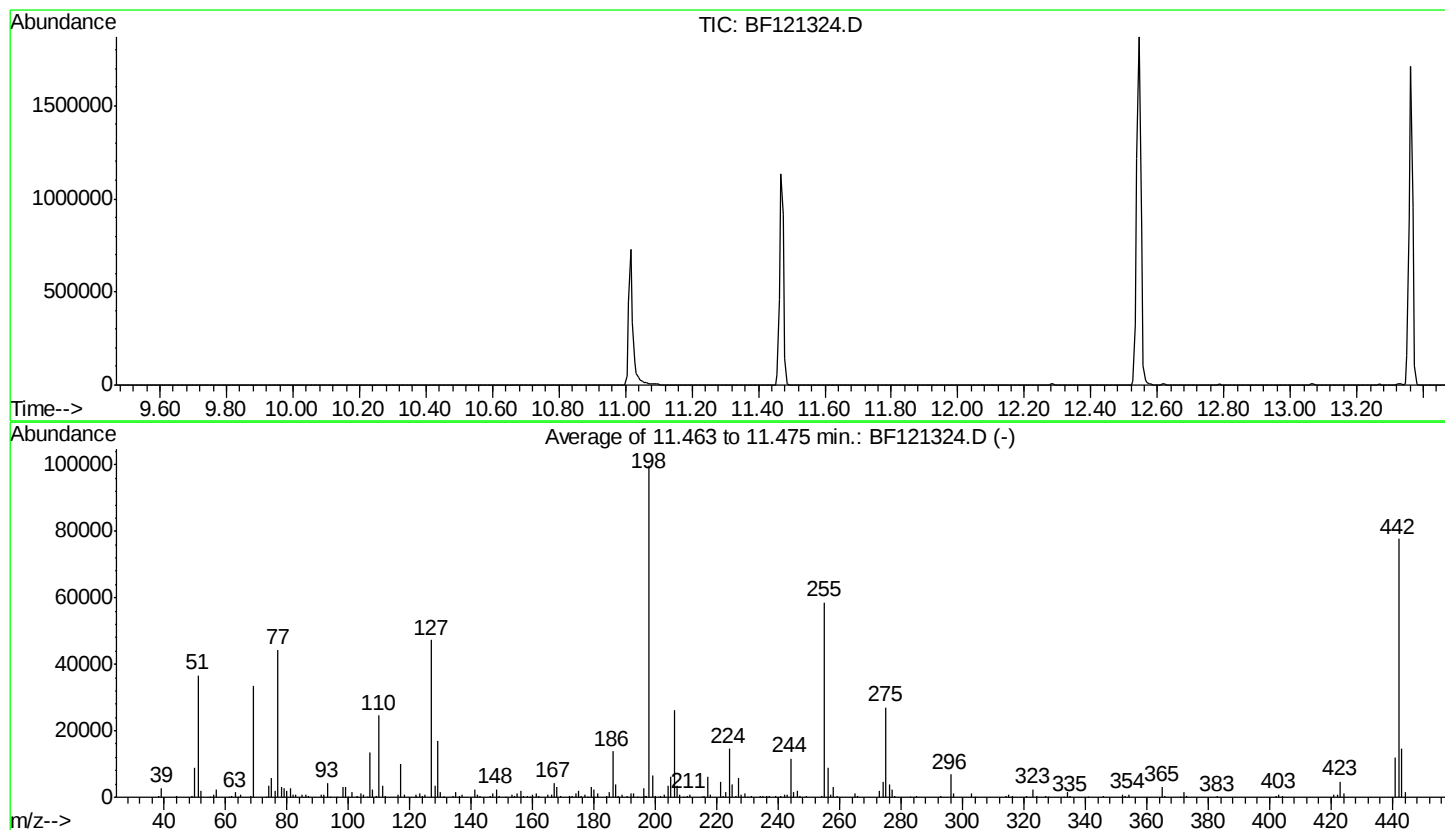

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	36634	PASS
68	69	0.00	2	1.5	497	PASS
69	198	0.00	100	33.7	33594	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	47314	PASS
197	198	0.00	2	0.4	350	PASS
198	198	100	100	100.0	99784	PASS
199	198	5	9	6.7	6690	PASS
275	198	10	60	27.2	27167	PASS
365	198	1	100	3.2	3182	PASS
441	198	0.01	100	12.2	12141	PASS
442	198	50	100	77.8	77666	PASS
443	442	15	24	18.6	14469	PASS